



**QUEEN'S
UNIVERSITY
BELFAST**

Evaluation of an alternative spectroscopic approach for aflatoxin analysis: Comparative analysis of food and feed samples with UPLC-MS/MS

Campbell, K., Ferreira Cavalcante, A. L., Galvin-King, P., Oplatowska-Stachowiak, M., Brabet, C., Metayer, I., Montet, D., Haughey, S. A., & Elliott, C. T. (2017). Evaluation of an alternative spectroscopic approach for aflatoxin analysis: Comparative analysis of food and feed samples with UPLC-MS/MS. *SENSORS AND ACTUATORS B-CHEMICAL*, 239, 1087-1097. <http://10.1016/j.snb.2016.08.115>

Published in:
SENSORS AND ACTUATORS B-CHEMICAL

Document Version:
Peer reviewed version

Queen's University Belfast - Research Portal:
[Link to publication record in Queen's University Belfast Research Portal](#)

Publisher rights

© 2016 Elsevier Ltd. This manuscript version is made available under the CC-BY-NC-ND 4.0 license <http://creativecommons.org/licenses/by-nc-nd/4.0/> which permits distribution and reproduction for non-commercial purposes, provided the author and source are cited.

General rights

Copyright for the publications made accessible via the Queen's University Belfast Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

The Research Portal is Queen's institutional repository that provides access to Queen's research output. Every effort has been made to ensure that content in the Research Portal does not infringe any person's rights, or applicable UK laws. If you discover content in the Research Portal that you believe breaches copyright or violates any law, please contact openaccess@qub.ac.uk.

Open Access

This research has been made openly available by Queen's academics and its Open Research team. We would love to hear how access to this research benefits you. – Share your feedback with us: <http://go.qub.ac.uk/oa-feedback>

Accepted Manuscript

Title: Evaluation of an alternative spectroscopic approach for aflatoxin analysis: Comparative analysis of food and feed samples with UPLC–MS/MS

Author: <ce:author id="aut0005" biographyid="vt0005" orcid="0000-0002-5994-2524"> Katrina Campbell Dr Ana L. Ferreira Cavalcante Pamela Galvin-King Michalina Oplatowska-Stachowiak Dr<ce:author id="aut0025" biographyid="vt0025" orcid="0000-0003-4434-908X"> Catherine Brabet Dr Isabelle Metayer Didier Montet Dr. Simon A. Haughey Dr. Christopher T. Elliott Prof.



PII: S0925-4005(16)31348-X
DOI: <http://dx.doi.org/doi:10.1016/j.snb.2016.08.115>
Reference: SNB 20796

To appear in: *Sensors and Actuators B*

Received date: 31-1-2016
Revised date: 30-6-2016
Accepted date: 19-8-2016

Please cite this article as: Katrina Campbell, Ana L.Ferreira Cavalcante, Pamela Galvin-King, Michalina Oplatowska-Stachowiak, Catherine Brabet, Isabelle Metayer, Didier Montet, Simon A.Haughey, Christopher T.Elliott, Evaluation of an alternative spectroscopic approach for aflatoxin analysis: Comparative analysis of food and feed samples with UPLC–MS/MS, *Sensors and Actuators B: Chemical* <http://dx.doi.org/10.1016/j.snb.2016.08.115>

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

Evaluation of an alternative spectroscopic approach for aflatoxin analysis: Comparative analysis of food and feed samples with UPLC-MS/MS

Katrina Campbell^{1*}, Ana L. Ferreira Cavalcante¹, Pamela Galvin-King¹, Michalina Oplatowska-Stachowiak¹, Catherine Brabet², Isabelle Metayer², Didier Montet², Simon A. Haughey¹, Christopher T. Elliott¹

¹ Institute for Global Food Security, School of Biological Sciences, Queen's University, David Keir Building Stranmillis Road, Belfast, UK BT95AG

² Centre de coopération Internationale en Recherche Agronomique pour le Développement, (CIRAD), UMR Qualisud, 73 rue Jean-François Breton, 34 398 Montpellier Cedex 5, France

*Corresponding author:

Dr Katrina Campbell

Tel: +44 (0) 28 90976535

Fax: +44 (0)28 90976513

E-mail: katrina.campbell@qub.ac.uk

Abstract

Increasing research has highlighted the effects of changing climates on the occurrence and prevalence of toxigenic *Aspergillus* species producing aflatoxins. There is concern of the toxicological effects to human health and animal productivity following acute and chronic exposure that may affect the future ability to provide safe and sufficient food globally. Considerable research has focused on the detection of these toxins, based on the physicochemical and biochemical properties of the aflatoxin compounds, in agricultural products for human and animal consumption. As improvements in food security continue more regulations for acceptable levels of aflatoxins have arisen globally; the most stringent in Europe. These regulations are important for developing countries as aflatoxin occurrence is high significantly effecting international trade and the economy. In developed countries analytical approaches have become highly sophisticated, capable of attaining results with high precision and accuracy, suitable for regulatory laboratories. Regrettably, many countries that are affected by aflatoxin contamination do not have resources for high tech HPLC and MS instrumentation and require more affordable, yet robust equally accurate alternatives that may be used by producers, processors and traders in emerging economies. It is especially important that those companies wishing to exploit the opportunities offered by lucrative but highly regulated markets in the developed world, have access to analytical methods that will ensure that their exports meet their customers quality and safety requirements.

This work evaluates the ToxiMet system as an alternative approach to UPLC-MS/MS for the detection and determination of aflatoxins relative to current European regulatory standards. Four commodities: rice grain, maize cracked and flour, peanut paste and dried distillers grains were analysed for natural aflatoxin contamination. For B1 and total aflatoxins determination the qualitative correlation, above or below the regulatory limit, was good for all commodities with the exception of the dried distillers grain samples for B1 for which no calibration existed. For B1 the quantitative R^2 correlations were 0.92, 0.92, 0.88 (<250 $\mu\text{g}/\text{kg}$) and 0.7 for rice, maize, peanuts and dried distillers grain samples respectively whereas for total aflatoxins the quantitative correlation was 0.92, 0.94, 0.88 and 0.91. The ToxiMet system could be used as an alternative for aflatoxin analysis for current legislation but some consideration should be given to aflatoxin M1 regulatory levels for these commodities considering the high levels detected in this study especially for maize and peanuts.

Keywords: ToxiMet, UPLC-MS/MS, Aflatoxin, food and feed, spectroscopy, Aflatoxin M1

Introduction

Aflatoxins, a group of mycotoxins first discovered after the occurrence of Turkey X disease in UK in the 1960s, are a most influential group of contaminants of concern for food security [1]. They are naturally occurring metabolites produced commonly by the toxigenic strains of the fungal species *Aspergillus* [2]. Several factors favour fungal growth including environmental, chemical and biological parameters. Two important factors affecting growth are the temperature and relative humidity with growth occurring between 10-35°C, optimally 30-35°C, and relative humidity optimally above 85% [3]. Due to an awareness of the risks of climate change to food security, increasing studies are emerging examining the role of climatic factors on specific fungal species and their gene expression for toxin production [4,5].

Aflatoxins are organic chemicals known as difuranocoumarins. They are classified into two broad groups according to their chemical structure; the difurocoumarocyclopentenone series (AFB1, AFB2, AFB2A, AFM1, AFM2, AFM2A and aflatoxicol) and the difurocoumarolactone series (AFG1, AFG2, AFG2A, AFGM1, AFGM2, AFGM2A and AFB3). The four major agriculturally important aflatoxins: B1, B2, G1, G2 were identified from their significant direct contamination of foods and feeds (Figure 1). These toxins have minor modifications in structure and molecular formulas and form a unique group of heat stable highly oxygenated, naturally occurring heterocyclic compounds. Aflatoxins B2 and G2 were established as the dihydroxy derivatives of B1 and G1, respectively. The aflatoxins display potency of toxicity, carcinogenicity, mutagenicity in the order of AFB1 > AFG1 > AFB2 > AFG2 [6]. Chemically the double bond of the dihydrofuran and the elements linked to the coumarin moiety are of importance in producing biological effects. The aflatoxins fluoresce strongly in ultraviolet light due to the ring structure (ca. 365 nm). The B label of aflatoxins B1 and B2 resulted from the exhibition of blue fluorescence under UV-light (425nm), while the G label refers to the yellow-green fluorescence of the relevant structures under UV-light (540nm). It has been reported that *Aspergillus flavus*, *Emericella astellata*, *E. venezuelensis* and *A. pseudotamarii* produce B1 and B2 while *A. parasiticus*, *A. nomius*, *A. bombycus*, *A. miniscleotigenes*, *A. arachidicola* produce B1, B2, G1 and G2 toxins [7]. The aflatoxins M1 and M2, two additional metabolic products were first isolated from milk of lactating animals fed aflatoxin preparations; hence, the M label [8]. Aflatoxin M1 is 4-hydroxy aflatoxin B1 and aflatoxin M2 is 4-dihydroxy aflatoxin B2 [9] and their toxic potency falls between B1 and G1 and B2 and G2 respectively.

Due to a combination of the optimal conditions required for fungal growth and susceptibility of the staple diets to *Aspergillus* growth these toxins tend to be most prevalent in tropical and subtropical regions, most of which are developing countries, causing severe negative impacts to food security [10, 11]. Since their identification the health and economic impacts of the occurrence, legislation and prevention of aflatoxin in feed and food have been well documented [12-19]. The most significant step was in 1993 when the International Agency for Research on Cancer (IARC) classified 'naturally occurring mixes of aflatoxins' as a Group 1 carcinogen, meaning that sufficient evidence exists to link aflatoxin exposure to cancer in humans [20]. Aflatoxin exposure leads primarily to a condition known as aflatoxicosis, a hepatic disease. Research suggests the exposure and susceptibility of individuals to aflatoxins from food contamination varies considerably depending on geographical location, type of diet, awareness of aflatoxin contamination, socioeconomic status, age, sex, nutritional status and/or concurrent exposure to other causative agents such as viral hepatitis (HBV) or parasite infestation. In animals, variations occur between species but aflatoxins are known to cause liver damage, anaemia, jaundice, gastrointestinal dysfunction, reduced feed utilization and efficiency with decreased milk and egg production, recurrent infection as a result of immunity suppression (e.g. salmonellosis), reduced reproductively and embryo toxicity in animals consuming low dietary concentrations. All ages are affected but to different degrees for different species with the young most susceptible. Nursing animals may be affected as a result of the conversion of aflatoxin B1 to the metabolite aflatoxin M1 excreted in milk.

To limit aflatoxin exposure, over 100 nations worldwide have set maximum tolerated levels of aflatoxin in food [21]. These standards offer public health protection in industrialized nations, but arguably have little effect in less developed countries through a lack of regulatory systems for aflatoxin monitoring and control. The US Food and Drug Administration has established specific guidelines on acceptable levels of aflatoxins in human food and animal feed by establishing action levels that allow for the removal of violative lots from commerce. In the US the action level for human food and cereals are 20 ppb total aflatoxins, with the exception of milk which has an action level of 0.5 ppb for aflatoxin M1. In Europe the maximum levels of aflatoxins for food consumption are generally lower as laid down in the Commission Regulation (EC) No 1881/2006, as amended by Commission Regulation (EU) No 165/2010 and Commission Regulation (EU) No 1058/2012 [22-24]. Therefore, the maximum levels for aflatoxin B1, the sum of aflatoxins B1, B2, G1 and G2 (known as Total) and aflatoxin M1 are

established therein varying with commodity and its use.

Aflatoxins have commonly been detected by their photo physical properties such as absorption and emission spectra. Recent developments in the detection and determination for aflatoxins have been reviewed highlighting the advantages and disadvantages between approaches [25]. In brief, the analysis of aflatoxins in food and feed includes chemically based analytical methods such as the AOAC thin layer chromatography method, capillary electrophoresis, high performance liquid chromatography or liquid chromatography coupled to mass spectrometry. These methods are primarily high cost requiring trained laboratory staff and facilities for accurate quantitative results. Non-invasive spectroscopy or hyperspectral imaging-based methods demonstrate potential for screening large samples contaminated with aflatoxins but cannot produce quantifiable results. Immunological methods such as enzyme linked immunosorbent assays, lateral flow devices and biosensor technology offer a low cost advantage but raise concerns in reliable repeatable detection and identification of individual toxin analogues. Due to the poor economic status and low education levels in developing countries, cost-effective quantifiable methods are required that will be easy to implement. The ToxiMet System first described in [26] has now been developed further, involving the introduction of new ToxiTrace and ToxiTrace cartridges and a substantially redesigned ToxiQuant instrument, a spectroscopic device which simultaneously identifies and quantitatively measures the individual aflatoxins by employing advanced spectroscopic and proprietary chemometric procedures. The device is constructed with the understanding that radiation of certain wavelengths excites certain mycotoxin contaminants such as aflatoxin to fluoresce. The wavelength of the emitted fluorescent light from the contaminant is significantly different (usually longer) than the excitation wavelength. On the theory that the amount of light emitted is proportional to the amount of the contaminant, a measurement of the amount of light emitted can be utilized to quantify the amount of target contaminant, such as aflatoxin, immobilized in a sample cartridge. Using the device involves the extraction of a contaminant such as aflatoxin from food, the immobilisation of the contaminant as a layer in a columnar packing, the illumination of the band, typically with UV radiation, at an applicable wavelength to excite the emission of fluorescent light by the band, the detection of the fluorescence and the conversion of the detected signal into a direct measurement of the concentration of the contaminant (typically in parts per billion) [27]. Therefore, the analytical sequence for the ToxiMet System is composed of four main steps: sample extraction; sample clean-up (using the ToxiSep cartridge); analyte immobilisation (on a ToxiTrace cartridge); followed by simultaneous measurement of the individual, immobilised toxins by the ToxiQuant instrument, without the need for chromatographic separation. The aim of the study was the comparative analysis of maize, rice and peanut samples and distillers grains for the determination of total aflatoxins

concentration and individual analogues B1, B2, G1 and G2 to determine the feasibility of the ToxiMet system relative to state of the art LC-MS/MS.

Materials and methods

Materials

Samples: Peanut paste (n=71), rice grains (n=88) and maize cracked and flour (n=79) samples (261-560 g each) used directly for human consumption were collected in the main markets of Abidjan, Bouaké and Korhogo in the Ivory Coast and kept at -20°C until sample preparation. Dried distillers grains (n=22) were sourced in Northern Ireland. All samples were analysed using both the Toximet System and UPLC-MS at the Institute for Global Food Security at Queen's University, Belfast.

Sample Preparation: Sample preparation was aimed at obtaining homogeneous samples. Frozen rice grain and cracked maize samples were milled in a grinder Retsch ZM 200 using a 1-mm sieve. The milled samples as well as the maize flour samples were homogenized during 30 minutes in a Chopin MR2L mixer. Peanut paste samples were thawed and homogenized during 15 minutes in a Thermomix VORWERK TM 21 by selecting the speed 2.5. The equipment was cleaned thoroughly between samples to prevent carry over contamination from sample to sample. Aliquots of the homogenized samples (70g) were kept at -20 °C until mycotoxin analysis and the same aliquot was used for both methods of analysis in the study.

ToxiMet System: ToxiSep and ToxiTrace cartridges were obtained from ToxiMet, UK. HPLC grade methanol, phosphate buffered saline (PBS) tablets (P4417) were purchased from Sigma Aldrich. Whatman No 41 and GF/A filter paper were obtained from GE Healthcare.

UPLC-MS/MS: LC-MS grade acetonitrile (ACN) (34967-2.5L); LC-MS grade methanol (34966-2.5L); formic acid for mass spectrometry 98 % (94318-50mL-F), ammonium hydroxide solution ≥25% in water (44273-100mL-F), magnesium sulphate ≥99.5% (M7506-500g), DMSO ≥99.9% (D8418-50mL) and amber vials (27000), Aflatoxins B2, G1, G2 and M1 were obtained from Sigma-Aldrich (Dorset, UK). Aflatoxin B1 was from Romer Labs (Tulln, Austria). A Bondesil C18 40 µm (29041013) was purchased from Agilent (Berkshire, UK). PTFE syringe filters (WHA67840402 Whatman Puradisc 4 syringe filter 0.2 µm PTFE) and polypropylene tubes (50mL and 15mL) (TPPA91051) were obtained from VWR. Sodium chloride (S/3120/53) was

obtained from Fischer chemicals. The water used was supplied from an in-house 18 M Ω Millipore water system, Millipore Ltd, (Hertfordshire, UK).

Methods

ToxiMet System Analysis

Sample extraction: Each sample (25g) was mixed with sodium chloride (2.5g) followed by the addition of deionised water (40mL) and blended for 2 minutes in a Sterilmixer 12 blender. The blender was cleaned thoroughly between each sample. Methanol HPLC Grade (60mL) was then added and blended into the mixture. The solution was filtered through Whatman No 41 filter paper and an aliquot of extract (20mL) was diluted with PBS solution (40mL) and mixed. This solution was then filtered through Whatman GF/A filter paper.

ToxiSep Clean Up Procedure: The ToxiSep cartridges were allowed to settle in an upright position for one hour at room temperature and positioned on a vacuum manifold. The red cap of the ToxiSep Aflatoxin cartridge was removed, the column tapped until the air bubbles dislodged and travelled to just underneath the frit. An air tight seal was formed. The lower cap was removed with the adaptor and reservoir fitted to the ToxiSep clean-up cartridge. An aliquot of the extract solution (24mL) was added slowly to the reservoir and allowed to pass through the ToxiSep cartridge at a flow of 3mL/min. The cartridge was then washed with PBS (20mL) at a flow of 5mL/min. Excess PBS was removed under high vacuum from the ToxiSep cartridge for 2-5 seconds. The retained aflatoxins were eluted into an amber volumetric flask (10mL) using methanol HPLC grade (1mL) followed by 1ml of water at a flow rate of 1 drop per second. The extract was diluted to 10ml on addition of water to the volumetric flask. The diluted elute was filtered through a 25mm syringe filter. The first 2mL was discarded into the waste beaker and the remainder collected into a 10ml amber flask.

ToxiTrace Immobilisation: The ToxiTrace cartridge was conditioned with methanol HPLC grade (0.2mL) followed by 10% methanol (0.2mL). An aliquot of the filtered sample extract (2.0mL) was loaded onto the column which was then washed using 10% methanol (0.4mL). The washing was complete when 50% of the solvent had passed through the cartridge.

Quantification: The Toxitrace cartridge was plugged and inserted into the ToxiQuant instrument (ToxiMet, UK) within one hour of preparation and analysed for aflatoxins by selecting the specific commodity from the on-screen menu. For dried distillers grains there was no specific option for the analysis of this sample type therefore these samples were analysed using the option of maize. The aflatoxin results B1, B2, G1, G2 and total aflatoxins are recorded for each sample immediately.

UPLC-MS/MS Analysis

Sample preparation: The sample preparation was based on the QUEChERS method [28,29] with some modifications [30]. Briefly, 1 g of homogenised sample was soaked with 5 mL of 2 % formic acid in water for 30 min followed by vortex mixing with 5 mL of acetonitrile using a DVX-2500 multi-tube vortexer set at a speed of 1000 for 30 min. The separation of the water from organic phase was achieved by addition of 2 g of magnesium sulphate and 0.5 g of sodium chloride and hand shaking for 30 sec followed by 5 min centrifugation at 4000g. The upper organic layer (2mL) was further purified by shaking for 30 sec with 0.1 g C18 silica sorbent and 0.3 g of magnesium sulphate. After centrifuging at 4000g for 1 min, an aliquot of extract (1mL) was transferred to a MS vial and DMSO (200 μ L) added. The solvent was evaporated off under nitrogen for approximately 45-60 min at room temperature. LC-MS/MS grade methanol (800 μ L) was added and the sample filtered using a 0.22 μ m filter.

Calibration: Matrix matched calibration curves were prepared with each batch of samples and used for calibration. Blank maize flour, rice flour and peanut paste samples previously tested and confirmed free from aflatoxins were used. An 8 point standard calibration curve in the range 0 to 50 μ g/kg is prepared by spiking known blank materials with aflatoxin working solutions before extraction.

UPLC-MS/MS: A Waters Acquity UPLC system coupled to Waters Xevo TQ-S triple quadrupole mass spectrometer was used (Waters, Milford, USA). The data were analyzed using TargetLynx software. The column used was CORTECS UPLC C18 1.6 μ m, 2.1 \times 100 mm (Waters, Milford, USA). The mobile phase A was 1 mM ammonium formate pH 6.5 in Milli-Q water and mobile phase B was 1 mM ammonium formate in methanol:acetonitrile (50:50). The gradient elution at a flow rate 0.4 mL/min started at 1 % mobile phase B and increased linearly to 99 % in 10

minutes, followed by 4 min equilibration. The injection volume was 1 μ L. The mass spectrometer was operated in the positive electrospray ionization mode and the parameters were as follows: capillary voltage 1.5 kV, source temperature 150°C, desolvation temperature 500°C, desolvation gas flow 1000 L/h. The MS/MS conditions for aflatoxins are presented in Table 1 and Figure 2 shows the retention time separation and multiple reaction monitoring (MRM) transitions of the 5 aflatoxins (B1, B2, G1, G2 and M1) using UPLC-MS/MS. The toxins were quantified by interpolation from a matrix-matched calibration curve (spiked before extraction so results were corrected for recoveries). For samples whereby the toxin concentration was above the upper calibration range these were diluted in blank matrix and re-analysed.

Results and discussion

As aflatoxins are reported to be genotoxic carcinogens, it is important to limit their total content in food and animal feed by complying with legislation for given commodities. Considering that European legislation includes limits for the most toxic aflatoxin B1 alone and the total aflatoxins (sum of aflatoxins B1, B2, G1 and G2) these are of primary focus for any method of analysis. On deciphering the ability of a method to be fit for purpose in a given environment a number of factors need to be considered including: accuracy; limit of detection; application to multiple analytes; versatility; time of analysis; cost; ease of use; low maintenance, repeatability and robustness. Key parameters were considered for both the ToxiMet system and UPLC-MS/MS instrument applied in this study (Table 2). The benefits of the ToxiMet system, compared with UPLC-MS/MS, included its ability to rapidly and simultaneously determine each of the individual aflatoxins, using unskilled personnel working outside of the laboratory environment. Additional benefits were the avoidance of the need for internal and analytical standards and low capital and maintenance costs as compared to the UPLC-MS/MS equipment. The benefit of the UPLC-MS/MS, in addition to being the regulatory method of choice, was the versatility to include other toxins within the analysis of the sample. Nonetheless, the individual determination of aflatoxins B1, B2, G1 and G2 in peanuts, maize, rice and distillers grain samples was shown to be feasible for both methods. The UPLC-MS/MS had the added ability of M1 determination (Supplementary Data). Table 3 summarises the range of the individual toxin concentrations determined by ToxiMet system

and UPLC-MS/MS analysis for each food and feed commodity. In general the upper limit of the range for the toxin concentration determined by UPLC-MS/MS was higher than for the ToxiMet system. Although the same lot was analysed by both methods these differences in range could be in part due to the variation in sample size from 1g to 25g taken from the lot as due to the heterogenic nature of mycotoxins this can be critical. Some of these challenges in sampling procedures to detect mycotoxins in agricultural commodities have been well described [31]. On each occasion the ToxiMet system provided an immediate result and did not indicate that the aflatoxin concentration was above an upper limit of detection. However, when the result was beyond the calibration range for UPLC-MS/MS analysis the sample was diluted and re-analysed on the instrument. Recent recommendations provided by the manufacturer since the completion of this study of evaluation of the instrument indicate that a very high levels for a quantitative as opposed to a qualitative result if the sample concentration is greater than 30 $\mu\text{g}/\text{kg}$ the sample should be diluted and re-analysed in the same manner as for UPLC-MS/MS. Figure 3 shows the graphical correlation of the results of the ToxiMet versus UPLC-MS/MS analysis for total aflatoxins (B1, B2, G1, G2) and for B1 determination in rice, maize, peanuts and dried distillers grains. The number and percentage of samples defined to be above the European regulatory limits for each sample type was compared between methods (Table 4).

Rice Samples: For rice included under the EU legislation 165/2010 whereby all cereals and all products derived from cereals, including processed cereal products have the limits of 2.0 $\mu\text{g}/\text{kg}$ for aflatoxin B1 and 4.0 $\mu\text{g}/\text{kg}$ for total aflatoxins (Sum of B1, B2, G1, G2). However, an exception is for AFB1 in processed cereal-based foods and baby food for infants and young children where the regulated limit is 0.1 $\mu\text{g}/\text{kg}$. Therefore, comparing the results from the ToxiMet system and UPLC-MS/MS analysis, 26 out of the 88 samples (29.5%) analysed by ToxiMet and 21 out of the 88 samples (23.9%) analysed by UPLC-MS/MS had their levels of aflatoxin B1 higher than the allowed legislation. For B1 analysis the variation arose in 5 samples (7RD2, 1RD3, 3RL3, 2RD4, 4RD4) which displayed results of 2.29, 2.48, 3.38, 2.15 and 2.24 $\mu\text{g}/\text{kg}$ by ToxiMet and 1.11, 1.13, 1.95, 1.16 and 1.43 $\mu\text{g}/\text{kg}$ by UPLC-MS/MS. For total aflatoxins 16 out of the 88 samples (18.2%) analysed by both ToxiMet system and UPLC-MS/MS were higher than the legislative limit. For total aflatoxins analysis the variation arose in four samples (2RL2, 3RL4,

9RL1, 1RL4) which displayed results of 2.24, 3.55, 4.08 and 5.05 µg/kg by ToxiMet compared to 4.61, 4.3, 3.21, and 3.88 µg/kg by UPLC-MS/MS respectively. As observed in Table 3 the range of aflatoxin concentrations and quantification in rice varies slightly between the two methods. The R^2 correlations of the concentrations determined for B1, B2, G1, G2 and total aflatoxins are 0.90, 0.45, 0.90, 0.54 and 0.92 (Supplementary data). For B2 and G2 the correlation was poor as the number of positive samples were low and bordering on the limit of quantification for both methods. The concentration range for aflatoxin M1 in the rice samples as determined by UPLC-MS/MS was 0 to 0.82 µg/kg with only 7 samples having measurable levels.

Maize Samples: For maize included under the EU legislation 165/2010 whereby all cereals and all products derived from cereals, including processed cereal products have the limits of 2.0 µg/kg for aflatoxin B1 and 4.0 µg/kg for total aflatoxins (Sum of B1, B2, G1, G2). Again, there is an exception for AFB1 in processed cereal-based foods and baby food for infants and young children where the regulated limit is 0.1 µg/kg. Therefore, comparing the results from the ToxiMet system and UPLC-MS/MS analysis, 40 out of the 79 samples (50.6%) analysed by ToxiMet and 36 out of the 79 samples (45.6%) analysed by LC-MS/MS had their levels of aflatoxin B1 higher than the allowed legislation. For B1 analysis the variation arose in eight samples (2M1, 3M2, 4M4, 2FP4, 4FP4, 3F4, 2M5, 2F5) which displayed results of 2.23, 0.35, 1.57, 1.53, 0.92, 1.72, 1.87 and 1.25 µg/kg by ToxiMet and 1.67, 4.21, 7.92, 2.02, 2.09, 3.13, 2.36 and 2.23 µg/kg by UPLC-MS/MS. For total aflatoxins 46 out of the 79 (58.2%) samples analysed by ToxiMet and 40 out of the 79 (50.6%) samples analysed by LC-MS/MS were higher than the legislative limit. For total aflatoxins analysis the variation arose in six samples (4M2, 3M2, 7M3, 2M5, 7FP5, 2F5) which displayed results of 5.59, 1.85, 3.43, 2.42, 2.96 and 3.96 µg/kg by ToxiMet and 3.11, 11.12, 4.33, 4.04, 5.29 and 7.17 µg/kg by UPLC-MS/MS. Most samples showing variability between the two methods were very close to the action level with the ToxiMet showing marginally lower levels overall compared to the MS method. The main discrepancies were in B1 and G1 values which were higher by UPLC-MS/MS. As observed in Table 3 the range of aflatoxin concentrations and quantification in maize varies at the upper limits of quantification. The R^2 correlations of the concentrations determined for B1, B2, G1, G2 and total aflatoxins in maize are 0.93, 0.51, 0.97, 0.77 and 0.94 (Supplementary data).

Similarly, for B2 and G2 the correlation was poor as the number of positive samples were low and bordering on the limit of quantification for both methods. The concentration range for aflatoxin M1 in the maize samples as determined by UPLC-MS/MS was 0 to 5.33 $\mu\text{g}/\text{kg}$ with 29 samples having measurable levels above the 0.05 $\mu\text{g}/\text{kg}$ EU level established for M1 in milk (Supplementary data).

Peanut Samples: The EU legislation for groundnuts (peanuts) and processed products thereof intended for direct human consumption or use as an ingredient in foodstuffs is 2 $\mu\text{g}/\text{kg}$ for aflatoxin B1 and 4 $\mu\text{g}/\text{kg}$ for total aflatoxins. The peanut samples were provided as a homogenate paste which was to be used for direct human consumption. For the analysis the peanut samples were the most difficult to handle. Both the rice and maize samples were a homogenised powder, and as such were easier to aliquot from the sample container. However, the buttery consistency of the peanut samples was troublesome and required more time for the ToxiMet system filtration step. As the extraction solvent was a 60% methanol solution the aflatoxins would be soluble and pass through the filter but the fats less soluble clogging the filter. Therefore, comparing the results from the ToxiMet system and UPLC-MS/MS analysis, 70 out of the 71 samples (98.6%) analysed by both methods had their levels of aflatoxin B1 higher than the allowed legislation and similarly their levels of total aflatoxins higher than the legislative limit. The same single sample was below legislative limits for both methods (1PA4). As observed in Table 3 the range of aflatoxin concentrations and quantification in peanut varies at the upper limits of quantification. The R^2 correlations of the concentrations determined for B1, B2, G1, G2 and total aflatoxins in peanuts are 0.22, 0.02, 0.005, 0.14 and 0.19 (Supplementary data). Although the qualitative comparison for peanuts was excellent relative to the legislative limit the correlation on quantification of the individual toxins was very poor due to samples with extremely high levels of aflatoxin contamination as determined by UPLC-MS/MS. As most samples were heavily contaminated it was impossible to examine the correlation relative to the low regulatory levels. When the quantitative R^2 correlation was performed for those samples with a total aflatoxins concentration below 250 $\mu\text{g}/\text{kg}$ the performance was much improved. The R^2 correlations of the concentrations determined for B1, B2, G1, G2 and total aflatoxins in peanuts for these samples was 0.88, 0.01, 0.90, 0.38 and 0.88. The most interesting point to note was the concentration range for aflatoxin M1 in

theses peanut samples as determined by UPLC-MS/MS was 0 to 381 $\mu\text{g}/\text{kg}$ with only 1 sample with no measurable M1 detected and all others well above the 0.05 $\mu\text{g}/\text{kg}$ level established for M1 in milk (Supplementary data).

Dried distillers grains: The EU legislation for dried distillers grains for use as an ingredient in animal feed is 20 $\mu\text{g}/\text{kg}$ for aflatoxin B1 and there is currently no regulation for total aflatoxins (Directive 2002/32/EC). Therefore, comparing the results from the ToxiMet system and UPLC-MS/MS analysis, none of the 22 samples analysed by ToxiMet or analysed by UPLC-MS/MS had their levels of aflatoxin B1 higher than the recommended EU legislation of 20 $\mu\text{g}/\text{kg}$. The R^2 correlations of the concentrations determined for B1, B2, G1, G2 and total aflatoxins in these samples was 0.91, 0.004, 0.47, 0.31 and 0.70 with levels detected by the ToxiMet system generally half of those detected by UPLC-MS/MS. The concentration range for aflatoxin M1 in these samples as determined by UPLC-MS/MS was 0 to 0.78 $\mu\text{g}/\text{kg}$ with only 5 samples having no measurable levels. It should be noted that for the dried distillers grains there was no choice for selection of dried distillers grains on the ToxiMet system as a commodity for analysis and as such the proprietary calibrations applied were not specific for this matrix. Therefore, the closest commodity of maize was chosen for the calibration and variations in matrix between maize and dried distillers grains could affect the performance for this commodity. Improved correlations may be obtained if the ToxiMet system is calibrated for this feed material.

The comparison of the testing platforms showed the key attributes, benefits and limitations (Table 2). For the food products collected from the Ivory Coast, the ToxiMet approach displayed a very good correlation with the state of the art confirmatory technique of UPLC-MS/MS for the qualitative detection of aflatoxin B1 and total aflatoxins at the European regulatory levels for these sample types. In relation to the quantification of aflatoxin there were significant discrepancies when the toxin levels were high as in the case of the peanut samples and for the B2 and G2 toxins. For the ToxiMet system there appeared to be no upper limit of detection and for all samples a concentration value was provided even if beyond the detection range. The variations in the B2 and G2 toxins may be due to the selectivity of the ToxiSep cartridge especially at high levels of total aflatoxins contamination. Additionally, at higher level of contamination the results might be underestimated as a portion of the aflatoxin target analytes might be lost during sample preparation when the ToxiSep cartridge reaches

its binding capacity. For the UPLC-MS/MS the use of the calibration curve showed the highly contaminated samples to be off scale and re-dilution was applied where necessary. Other discrepancies in quantification can arise in the homogeneity of the sample mass analysed, the efficiency of the extraction procedures and in the preparation of the analytical standards for the UPLC-MS/MS method. Although the sample was milled and thoroughly mixed the ToxiMet system utilised a more representative 25g compared to 1g by the UPLC-MS/MS method reducing the potential for toxin hotspots. Generally, the correlation trend of the UPLC-MS/MS method to the ToxiMet system is that the UPLC-MS/MS method detected higher levels of B1 and total aflatoxins. Extraction procedures with multiple steps allow for error and for untrained personal the methods should be as simple as possible. Both methods have solvent based extraction steps with multiple steps for the operator though the ToxiMet system uses only methanol as a solvent and overall is a relatively faster procedure. A major advantage of the ToxiMet system is that analytical standards are not required. For the preparation of calibration standards precision is required for highly sensitive detection methods as even small error margins through solvent evaporation of the stock standard on preparation, storage or pipetting can cause differences in response at the low levels of detection which can amplify to significant differences in the toxin concentration in the sample. The use of internal standards for mass spectrometry procedures would be the preferable option for precision analysis though to date these are only available for certain analytes for mycotoxin analysis and are highly expensive for routine use.

The samples collected in this study from the Ivory Coast were for direct human consumption in the local community. These samples showed high levels of contamination of aflatoxins well above the European regulatory limits in the order of severity of peanuts, maize and rice. To prevent adverse human health effects from high levels of aflatoxin contamination food choices in this region may be an important aspect whereby rice may have less risk for toxic concerns due to the occurrence determined in this study. Innovative cost effective detection can offer a means of prevention of contaminated products entering into the food chain but in regions where food supply is more important than safety from chronic toxin exposure, research and innovation must examine strategic mitigation strategies to ensure sufficient food supply. Limitations of both methods currently lie in their ability to detect AFB1 in processed cereal-based foods and baby food for infants and young children at the regulated limit is 0.1 µg/kg as the

LODs for B1 using the method are currently 0.5 µg/kg for UPLC-MS/MS and 0.2 µg/kg for ToxiMet. This would potentially pose issues for these commodities unless minor modifications to the sample preparation can be considered for increased sensitivity. Another current limitation of the ToxiMet system is that it currently does not detect aflatoxin M1 or as in comparison to advanced LC-MS/MS methods the simultaneous detection of other mycotoxins. The presence of aflatoxin M1 in maize samples highly contaminated with aflatoxin B1 has been reported previously [32]. Similarly Huang and co-workers [33] found aflatoxins M1 and M2 in peanuts with the highest content 64.7 and 3.6 µg/kg, respectively. This study highlights in agreement with previous authors that aflatoxin M1 is not only an important contamination concern of milk but that regulation should also be considered for foodstuffs such as peanuts and maize.

Conclusion

The ToxiMet system provides an alternative significantly lower cost approach compared to mass spectrometry analysis in both instrumentation and maintenance costs and day to day operation of the assay that would be useful for the prevention of highly contaminated foodstuffs with aflatoxins entering the food chain. This type of technology could be suitable for use as a highly accurate food safety monitoring tool in trading, distributing and processing companies in emerging economies where contamination in key staple foods and major export crops can be high as illustrated in this study for maize and peanut samples. Such a system can be useful in laboratories for the determinations and removal of contaminated lots where there are limited resources for highly expensive analytical equipment and trained staff. In agreement with Yao et al 2015 an integrated approach which incorporates rapid sample screening techniques with analytical methods may be most suitable for detecting aflatoxins in consumables. A recommendation for future consideration is for the ToxiMet technology to undergo a full inter-laboratory trial with the inclusion of certified reference materials against other techniques. Though the inclusion of both methods of analysis in proficiency testing schemes would help determine further the accuracy of each technique especially at key regulatory levels.

Acknowledgements

This research was funded through the Advanced ASSET project, partly funded through InvestNI and the European Sustainable Programme 2007-2013 under the European Regional Development Fund. The authors would like to acknowledge the EuropeAid project 3CIvoire which funded sample collection in the Ivory Coast, preparation of the samples and shipment to Queen's University Belfast for analysis. The authors would like to thank both Laurine Engrand from the Graduate School of Life Sciences of Toulouse ENSAT in France and Elise Lapie from Lasalle Beauvais Polytechnic Institute, France for the contributions to this work during their student placement at the Institute for Global Food Security.

References

1. Richard JL (2008) Discovery of aflatoxins and significant historical features. *Toxin Reviews*, 27 (3-4) 171-201
2. Da Costa CL, Geraldo MRF, Arroiteia CC, Kemmelmeier C (2010). In vitro activity of neem oil on *Aspergillus flavus* growth, sporulation viability of spores, morphology and aflatoxin B1 and B2. *Advances in Biosciences and Biotechnology* 1: 292-299.
3. Shehu K and Bello MT (2011) Effect of Environmental Factors on the Growth of *Aspergillus* Species Associated with Stored Millet Grains in Sokoto. *Nigerian Journal of Basic and Applied Science*, 19(2):218-223
4. Ehrlich KC, Montalbano BG and Cotty PJ (2003) Sequence comparison of aflR from different *Aspergillus* species provides evidence for variability in regulation of aflatoxin production. *Fungal Genetics and Biology* 38: 63-74.
5. Medina A, Rodríguez A, Sultan Y and Magan N (2015) Climate change factors and *Aspergillus flavus*: effects on gene expression, growth and aflatoxin production *World Mycotoxin Journal*, 8 (2): 171-179
6. Carnaghan RB, Hartley RD, O' Kelly J (1963) Toxicity and fluorescence properties of the aflatoxins. *Nature*, 200, 1101.
7. Razzaghi-Abyaneh M, Shams-Ghahfarokhi M, Peng-Kuang C (2010) Aflatoxins: Mechanism of inhibition by antagonistic plants and bacteria. (Eds) www.intechopen.com/books/...586-304.
8. De Longh H, Vles Ro, Van Peltj (1964) Milk of mammals fed an aflatoxin-containing diet. *Nature* 202, 466
9. Holzapfel CW, Steyn PS, Purchase IF (1966) Isolation and structure of aflatoxins M1 and M2. *Tetrahedron Letters* 25, 2799
10. Strosnider H, Azziz-Baumgartner E, Banziger M, Bhat RV, Breiman R, Brune MN, DeCock K, Dilley A, Groopman J, Hell K, Henry SH, Jeffers D, Jolly C, Jolly P, Kibata GN, Lewis L, Liu X, Lubber G, McCoy L, Mensah P, Miraglia M, Misore A, Njapau H, Ong CN, Onsongo MT, Page SW, Park D, Patel M, Phillips T, Pineiro M, Pronczuk J, Rogers HS, Rubin C, Sabino M, Schaafsma A, Shephard G, Stroka J, Wild C, Williams JT, Wilson D. (2006) Workgroup report: public health strategies for reducing aflatoxin exposure in developing countries. *Environmental Health Perspectives*; 114(12):1898–1903.
11. Enyiukwu D.N., Awurum A.N., Nwaneri J.A. (2014) Mycotoxins in Stored Agricultural Products: Implications to Food Safety and Health and Prospects of Plant-derived Pesticides as Novel Approach to their Management *Greener Journal of Microbiology and Antimicrobials*, 2 (3), 32-48

12. Miller JD (1999). Fungi and mycotoxins in grain: implications for stored products research. Proceedings of the 6th international Working Conference on Stored Product Research. 2, 971-977.
13. Williams JH, Phillips TD, Joll PE, Stiles JK, Jolly CM and Aggarwal D (2004) Human aflatoxicosis in developing countries: a review of toxicology, exposure, potential health consequences and interventions. American Journal of Clinical Nutrition 80 (5), 1106-1122
14. Khlangwiset P and Wu F (2010) Costs and efficacy of public health interventions to reduce aflatoxin-induced human disease. Food Additives and Contaminants Part A Chemical Analysis Control and Exposure Risk Assessment 27 (7) 998-1014.
15. Wild CP, Gong YY (2010) Mycotoxins and human disease: a largely ignored global health issue. Carcinogenesis 31 (1) 71-82
16. Reddy KRN, Salleh B, Saad B, Abbas HK, Abel CA, Shier WT (2010) An overview of mycotoxin contamination in foods and its implications for human health . Toxin Reviews 29 (1) 3-26
17. Marin S, Ramos A.J., Cano-Sancho G., Sanchis V (2013) Mycotoxins: Occurrence, toxicology, and exposure assessment Food and Chemical Toxicology 60, 218–237
18. Razzaghi-Abyaneh M, Chang PK, Shams-Ghahfarokhi M and Rai M. (2014) Global health issues of aflatoxins in food and agriculture: challenges and opportunities. Frontiers in Microbiology, 5 (420) 1-3
19. Wu F. (2015) Global impacts of aflatoxin in maize: trade and human health. World Mycotoxin Journal, 8 (2): 137-142
20. International Agency for Research on Cancer (IARC), 1993. IARC Monographs on the Evaluation of Carcinogenic Risks to Humans: Some Naturally Occurring Substances: Food Items and Constituents, Heterocyclic Aromatic Amines and Mycotoxins. IARC Scientific Publications No. 56, IARC, Lyon, France.
21. CAST (2003) Mycotoxins: risks in plant, animal, and human systems. Ames, Iowa: Council for Agricultural Science and Technology.
22. Commission Regulation (EC) No 1881/2006 of 19 December 2006 setting maximum levels for certain contaminants in foodstuffs. Official Journal of the European Union L364/5
23. Commission Regulation (EU) No 165/2010 of 26 February 2010 amending Regulation (EC) No 1881/2006 setting maximum levels for certain contaminants in foodstuffs as regards aflatoxins. Official Journal of the European Union L50/8
24. Commission Regulation (EU) No 1058/2012 of 12 November 2012 amending Regulation (EC) No 1881/2006 as regards maximum levels for aflatoxins in dried figs. Official Journal of the European Union L313/14

25. Yao H, Hruska Z, Diana Di Mavungu, J (2015) Developments in detection and determination of aflatoxins. *World Mycotoxin Journal*, 8 (2): 181-191
26. Piletska E, Karim K, Coker R, Piletsky S (2010) Development of the custom polymeric materials specific for aflatoxin B1 and ochratoxin A for application with the ToxiQuant T1 sensor tool. *Journal of Chromatography A*, 1217 (2010) 2543–2547
27. Coker RD, Nagler MJ, Andreou MP (2006) Device for detection and measurement of a target compound such as a food toxin Patent number WO 2006123189 A2
28. Lacina, O., Zachariasova, M., Urbanova, J., Vaclavikova, M., Cajka, T., Hajslova, J. (2012) Critical assessment of extraction methods for the simultaneous determination of pesticide residues and mycotoxins in fruits, cereals, spices and oil seeds employing ultra-high performance liquid chromatography-tandem mass spectrometry, *Journal of Chromatography A*, 1262, 8-18.
29. Dzuman Z, Zachariasova M, Lacina O, Veprikova Z, Slavikova P, Hajslova J (2014) A rugged high-throughput analytical approach for the determination and quantification of multiple mycotoxins in complex feed matrices, *Talanta*, 121, 263-272
30. Oplatowska-Stachowiak M, Haughey SA, Chevallier O, Galvin-King P, Campbell K, Magowan E, Adam G, Berthiller F, Krska R, Elliott CT (2015) The determination of mycotoxin content in dried distillers grain with solubles (DDGS) using a multianalyte UPLC-MS/MS method: Implications for the safe use of this alternative energy source in animal feeds. *Journal of Agricultural and food chemistry* DOI: 10.1021/acs.jafc.5b03844
31. Whitaker TB, Slate AB, Doko MB, Maestroni BM, Cannavan A. Sampling procedures to detect mycotoxins in agricultural commodities 2011 Springer Netherlands
32. Shotwell OL, Goulden ML, Hesseltine CW (1976) Aflatoxin M1. Occurrence in stored and freshly harvested corn. *Journal of Agricultural and Food Chemistry*, 24 (3), 683-684
33. Huang B, Han Z, Cai Z, Wu Y, Ren Y (2010) Simultaneous determination of aflatoxins B1, B2, G1, G2, M1 and M2 in peanuts and their derivative products by ultra-high-performance liquid chromatography-tandem mass spectrometry. *Analytica Chimica Acta*, 662, 62-68

Biographies for publication

Dr Katrina Campbell is a Lecturer in Bioanalytical Systems and heads the Biosensors Strand within the Centre for ASsured, SafE and Traceable food (ASSET). Katrina is a member of the Royal Society of Chemistry and the Royal Institute of Biology. Katrina obtained a BSc (Hons) in Biochemistry in 1995; a MMedSc in Ultrastructural Anatomy and Pathology in 1996 and PhD in Pharmacy focusing on novel systems for transdermal drug delivery in 2001 from Queen's University Belfast. Until 2012 she was employed as a post-doctoral research fellow for Queen's University in developing innovative screening methods for the detection of chemical contaminants and toxins in food, animal feeds and the environment. She has extensive experience in bioanalytical method development, validation and evaluation with state of the art technologies, end product formation as kits and technology transfer workshops and events for dissemination. Her research focuses on the identification and recognition of known and emerging threats within the entire food supply chain from “environment to farm to fork” and to determine their consequential effects.

Ana Ferreira Cavalcante was an undergraduate one year placement student on the Food Quality, Safety and Nutrition Degree Pathway at Queen's University Belfast. She commenced her studies at the Universidade Estadual de Campinas in Sao Paulo and was funded by the Brazilian Science without Border Programme sponsored by their Ministry of Education (MEC - CAPES) and the Ministry of Science and Technology (MCT - CNPq) to undertake her placement.

Pamela Galvin King obtained her BSc. 2.1 Honours degree in Equine Science in 2004 and her MSc on the Comparison of Diagnostic Methods for the Diagnosis of Equine Influenza in 2013 both from the University of Limerick. She was employed as a research technician at the Institute for Global Food Security, Queen's University Belfast in 2012. She is involved in a range of studies on the rapid detection of mycotoxins, heavy metals and food fraud through method development and/or analysis by carrying out extractions and data analysis. She is currently in the first year of a part time PhD programme to develop rapid methods to detect economically motivated adulteration in the herb and spice industry.

Dr Michalina Oplatowska-Stachowiak obtained an MSc in Biotechnology at the Technical University of Lodz, Poland in 2007 and a PhD specialising in the immunochemical techniques for the detection of food contaminants from Queen's University, Belfast (QUB) in 2010. She was since employed as a Research Fellow at the Institute for Global Food Security at QUB on projects that focused on the development and validation of immunochemical and LC-MS/MS methods for the detection of food and feed contaminants.

Dr Catherine Brabet received the PhD in Food Science from the University of Montpellier (France) in 1994. She has 14 years' experience of R&D in the southern countries: 3 years at CIAT (International Center for Tropical Agriculture) in Colombia, 3 years at CIP (International Potato Center) in Peru, 7 years at the UNICAMP (Universidade Estadual de Campinas) in Brazil and one year at UAC (Université d'Abomey-Calavi) ex UNB (Université Nationale du Bénin) in Benin. Since 2001, she has been working as a researcher in food safety and quality at CIRAD (Centre de coopération internationale en recherche agronomique pour le développement), Montpellier, France. Her main research activities concern the prevention and control of mycotoxins in foods, and plant pathogenic fungi, including the development and validation of rapid methods for mycotoxin analysis.

Isabelle Piro-Metayer has been working as technician at CIRAD since 1982 (Centre de coopération internationale en recherche agronomique pour le développement), Montpellier, France. As member of the food safety team of the UMR Qualisud, she has been involved in the management of the laboratories and in the research within national and international projects (eg EU projects such as Inco-Dev Mycotox, EuropeAid 3Civoire...) by supporting the analytical activities (sample preparation and microbiological, molecular and mycotoxin analyses).

Dr. Didier Montet leads the team of Control of contaminants along the food chain (food safety team) at CIRAD in Montpellier, France. He was awarded his Ph.D. in Food microbiology in 1984 at the University of Montpellier. He is also vice-chair of Biotechnology group at the National French Agency

for food-safety (Anses). His main research topic concerns the understanding of the microbial ecology of food and food-safety. He has published nearly 130 papers in the field of food. He currently runs a Europe Aid Project in Côte d'Ivoire and participates in different European projects. He was food expert for the French Embassy in south-east Asia and was professor at the Asian Institute of Technology in Thailand (1997-1999).

Dr. Simon Haughey is a Senior Research Fellow within the Institute for Global Food Security at Queen's University Belfast and is the manager of the ASSET Technology Centre. He has a B.Sc. (Hons) in Pure and Applied Chemistry and a PhD in Organic Chemistry. He has published more than 50 scientific papers. He spent more than 8 years as a Senior Research Scientist in industry where his activities included research, product development and manufacturing of *in vitro* diagnostic kits for use on SPR technology. His current research interests include spectroscopic fingerprinting techniques (e.g. RAMAN/NIRS/FT-IR) and food/feed quality and safety, food/feed authenticity/fraud/provenance.

Prof Christopher Elliott is *Pro Vice Chancellor for the Faculty of Medicine, Health & Life Sciences*, Professor of Food Safety and founder of the Institute for Global Food Security at Queen's University Belfast. He has published more 300 peer review articles, many of them relating to the detection and control of agriculture, food and environmental related contaminants. His main research interests are in the development of innovative techniques to provide early warning of toxin threats across complex food supply systems. Protecting the integrity of the food supply chain from fraud is also a key research topic and Chris led the independent review of Britain's food system following the 2013 horsemeat scandal. Over the years Chris has developed a high level network of collaborators through co-ordinating and participating in multiple European framework research projects. He is a founding member of the International School for Advanced Residue Analysis in Food based in France and a visiting Professor at the China Agriculture University in Beijing and the Chinese Academy of Sciences, a recipient of a Winston Churchill Fellowship and an elected Fellow of the Royal Society of Chemistry, Royal Society of Biology and the Institute of Food Science and Technology.

Figure 1: Structures of aflatoxin analogues

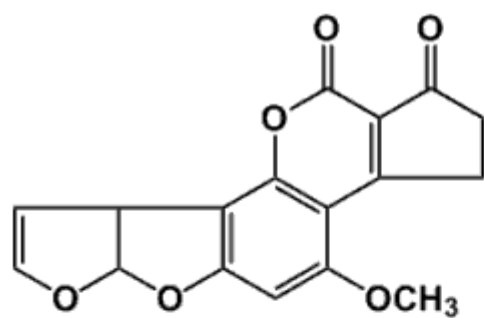
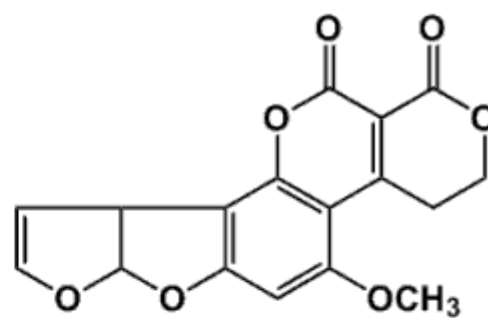
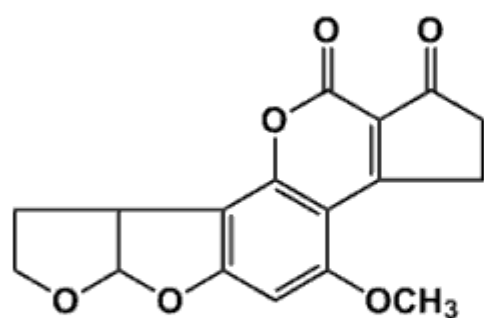
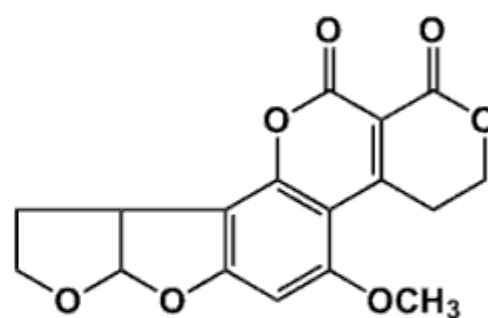
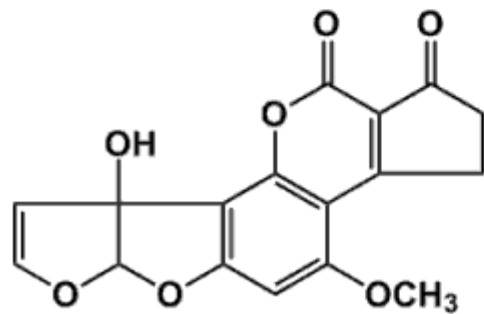
Aflatoxin B₁Aflatoxin G₁Aflatoxin B₂Aflatoxin G₂Aflatoxin M₁

Figure 2. Retention time separation and multiple reaction monitoring (MRM) transitions of the 5 aflatoxins (B1, B2, G1, G2 and M1) using UPLC-MS/MS.

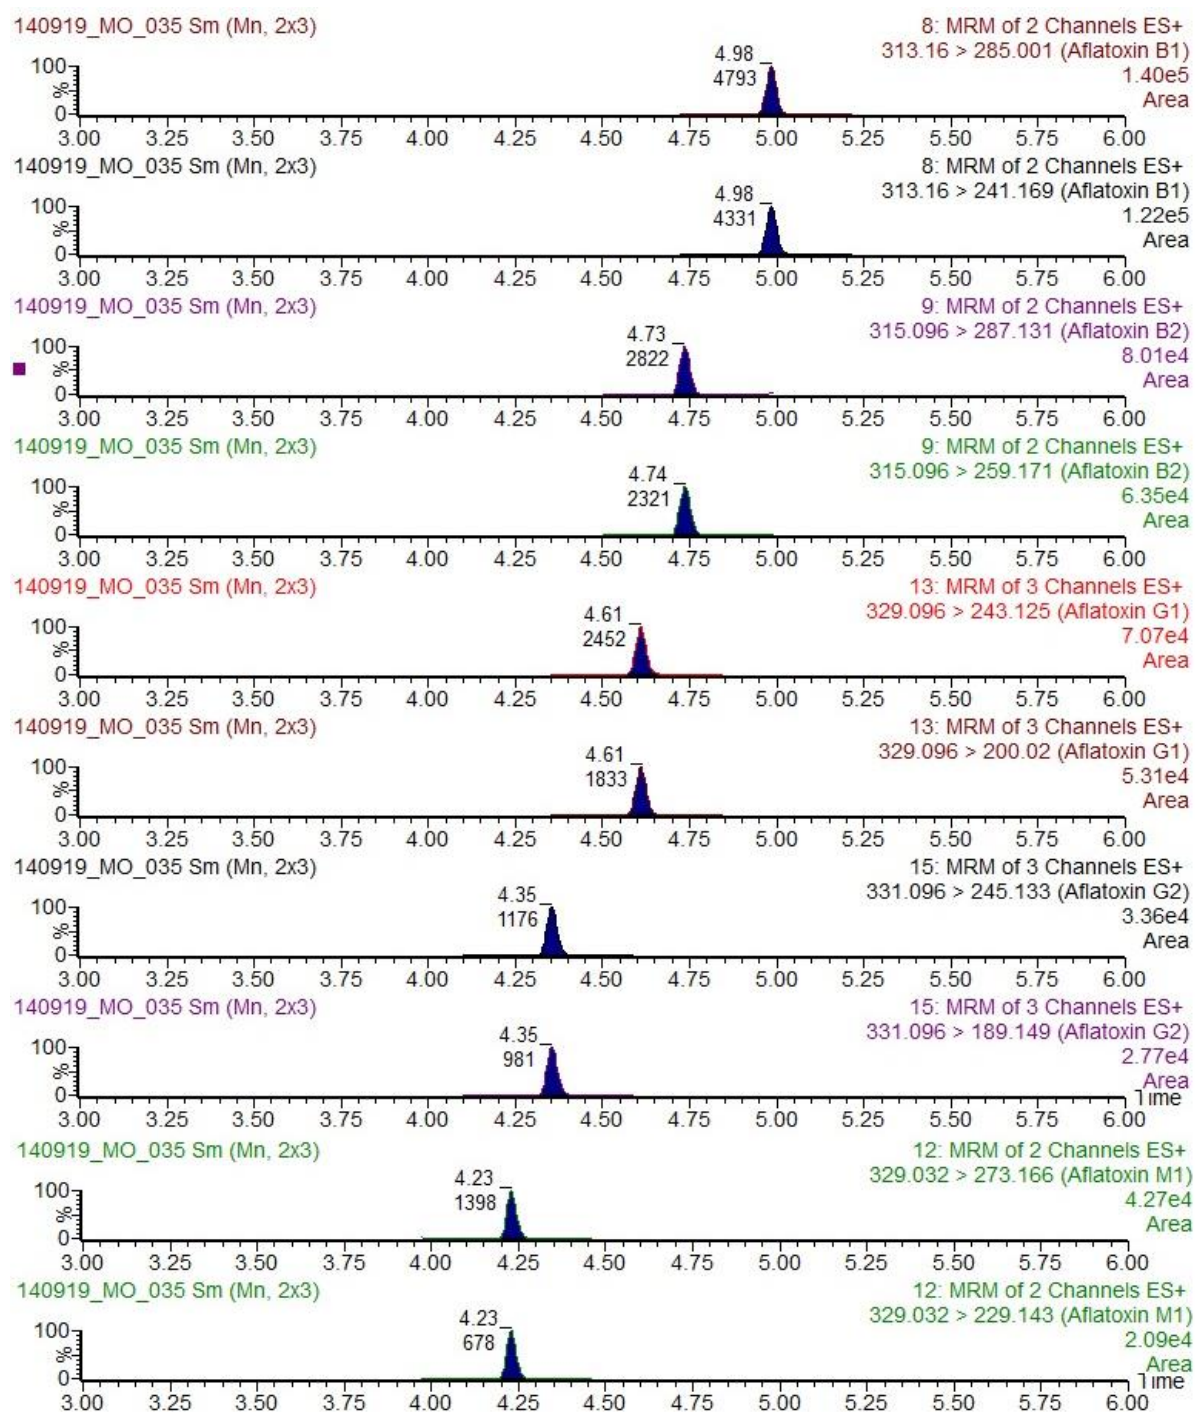
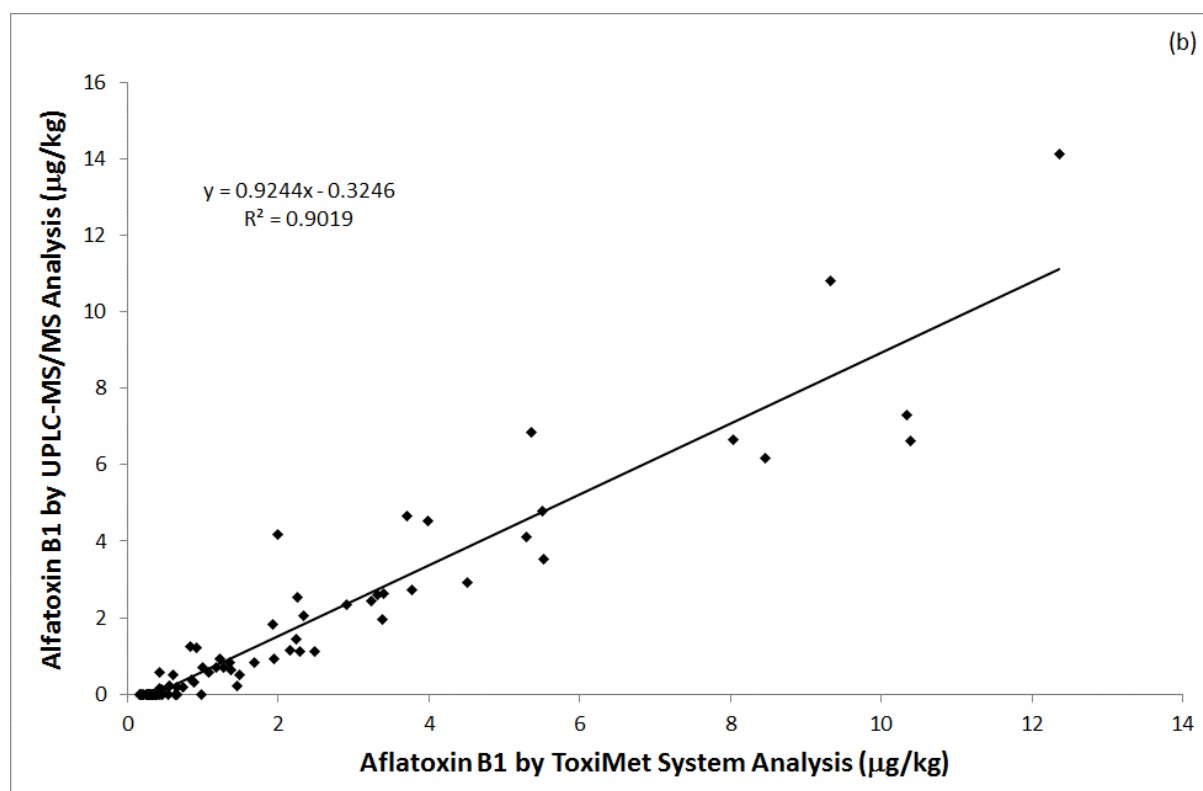
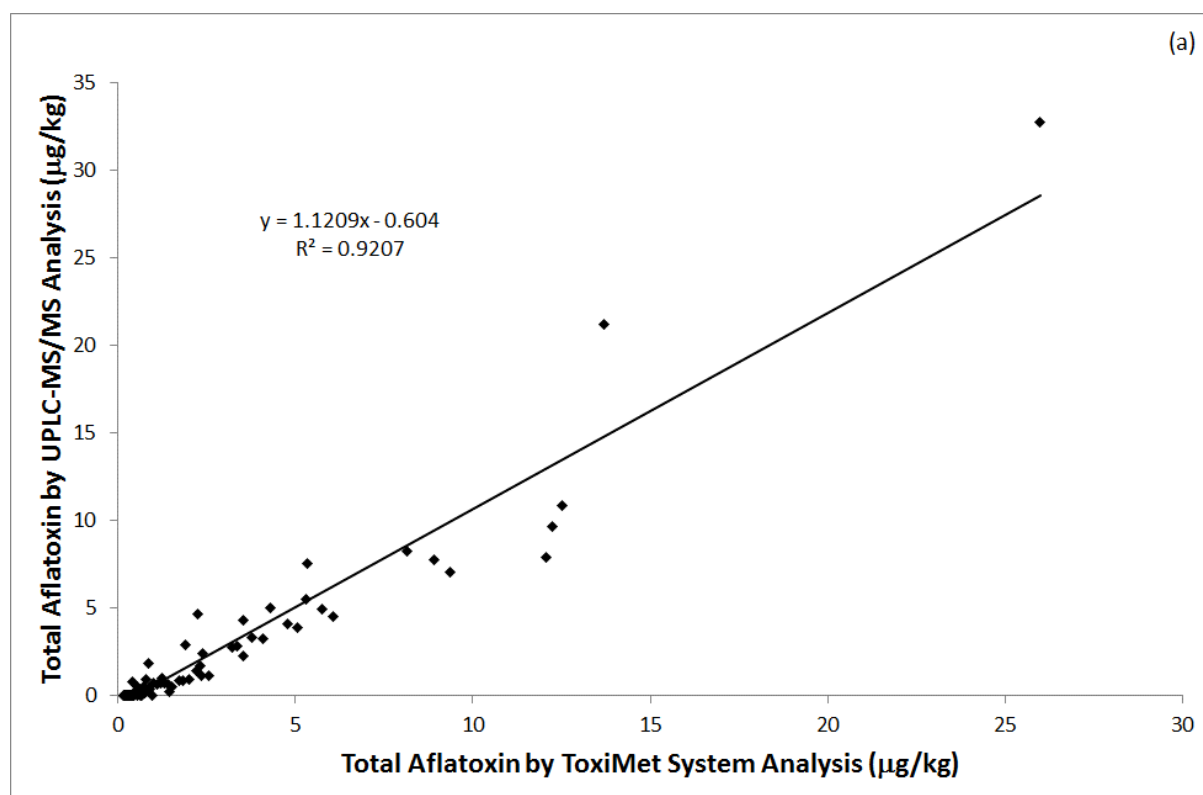
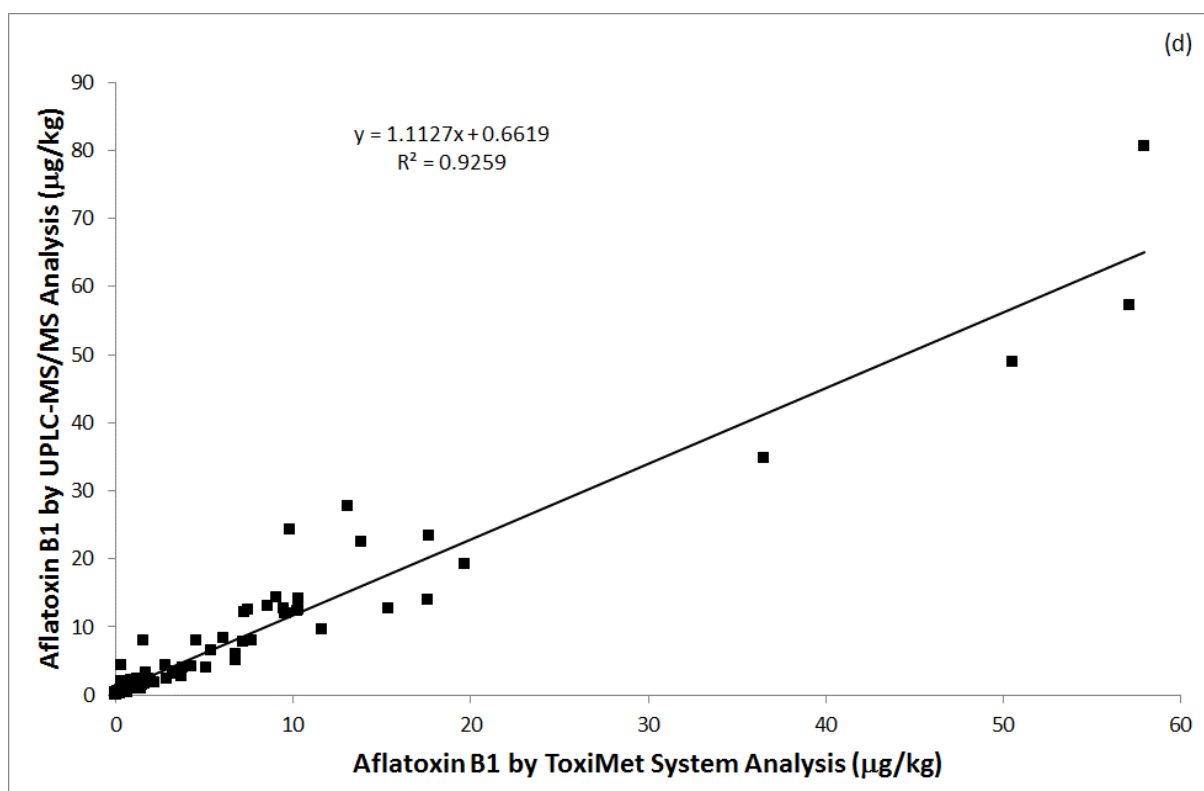
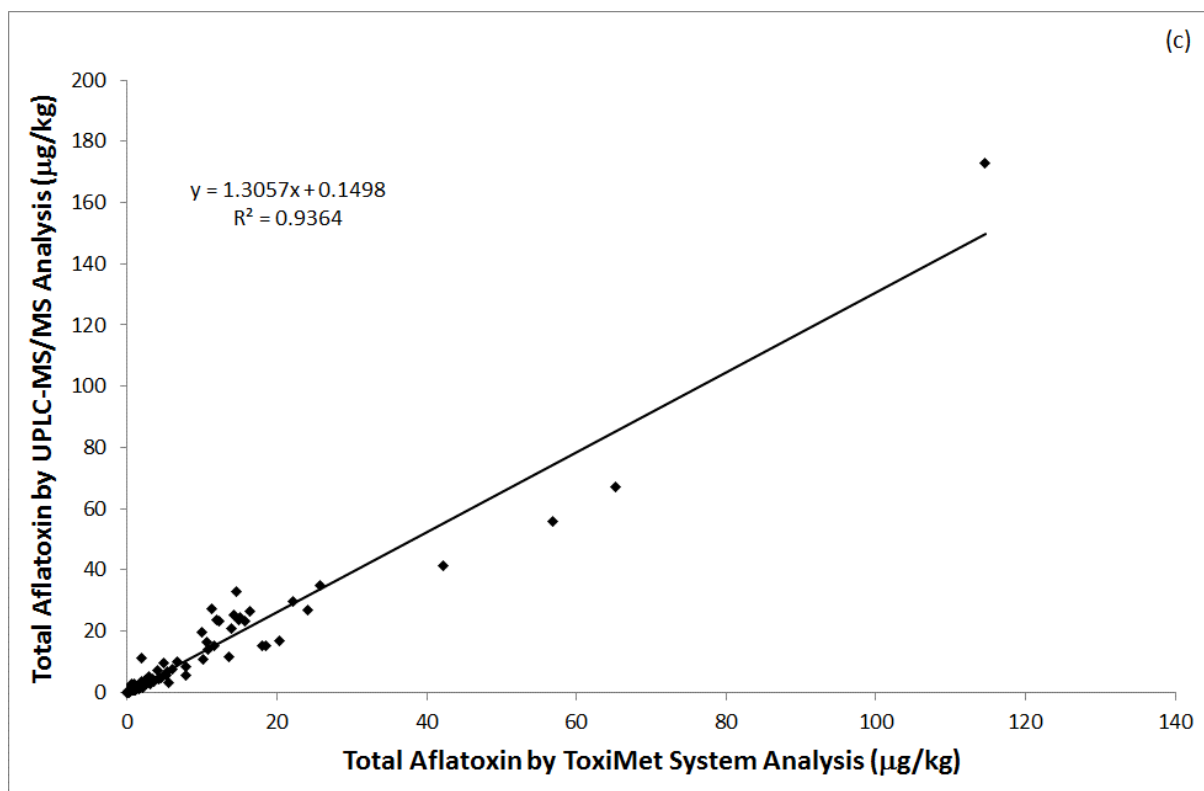
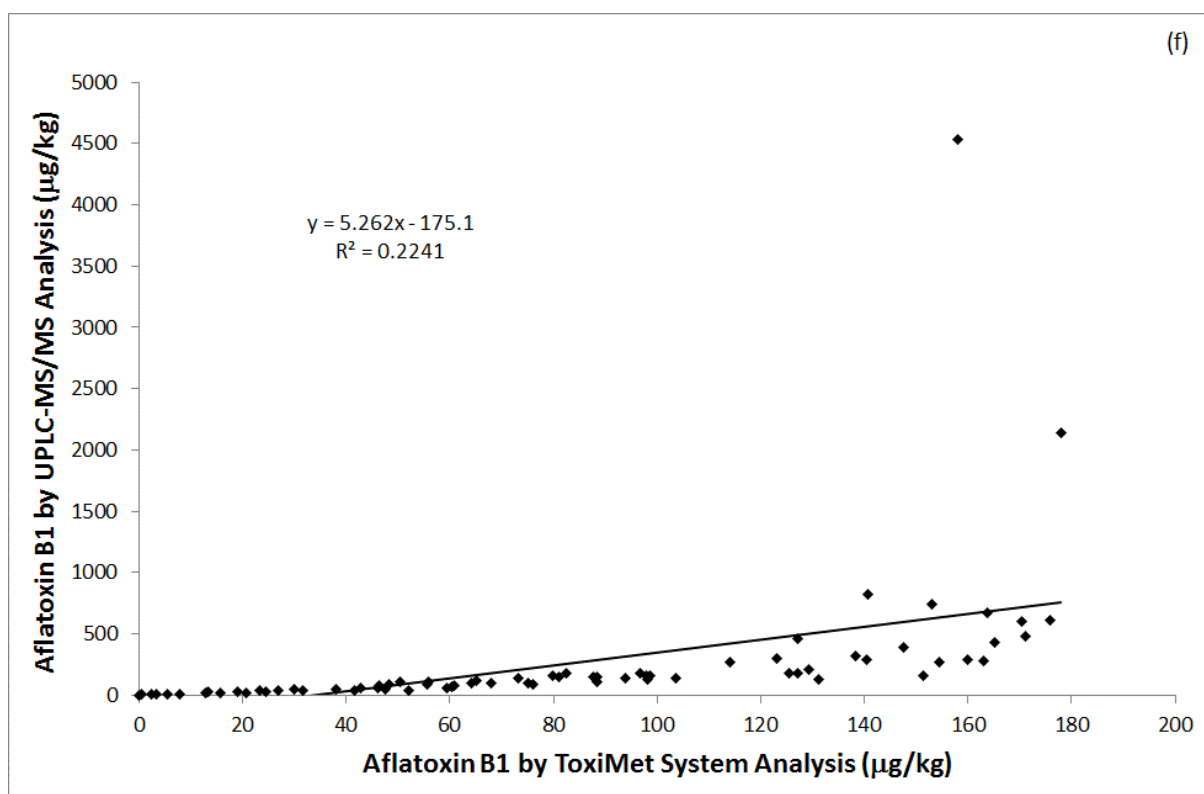
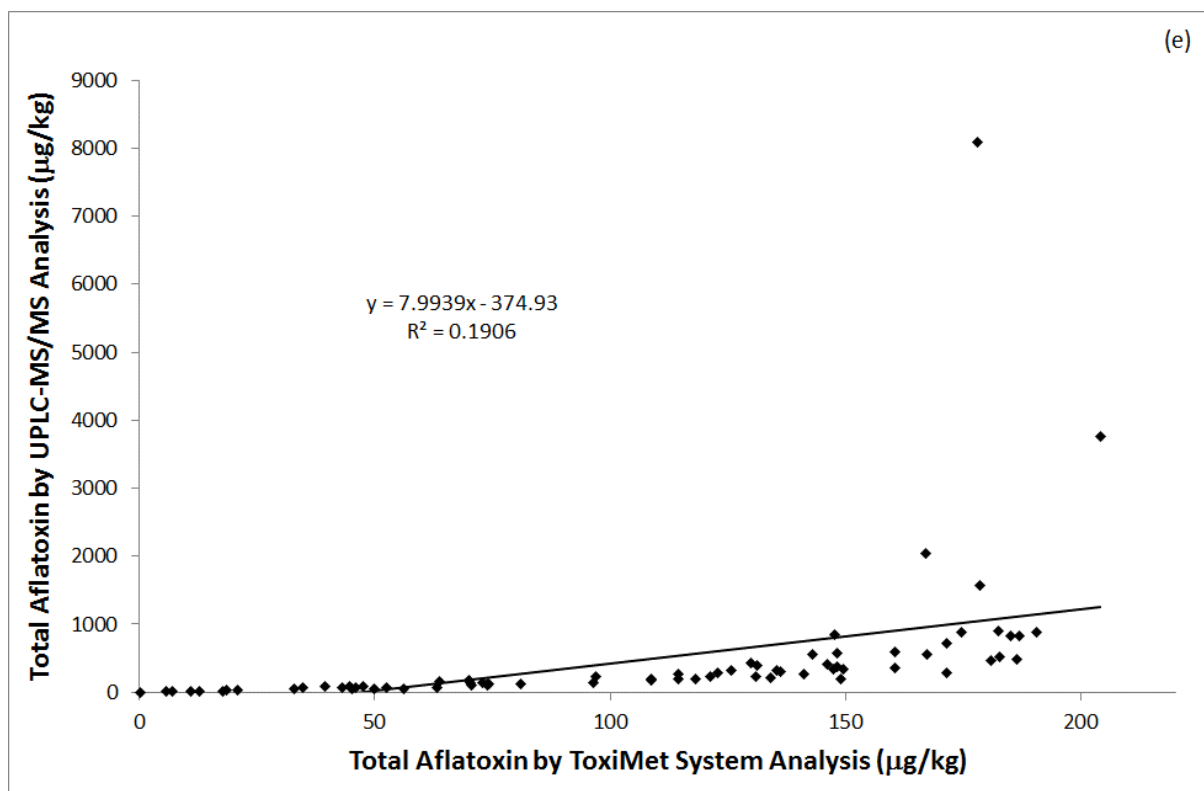


Figure 3: Comparison of UPLC-MS/MS and ToxiMet System Analysis total aflatoxins (B1, B2, G1, G2) and B1 determination in rice (a, b), maize (c, d), peanuts (e, f) and dried distillers grain (g, h).







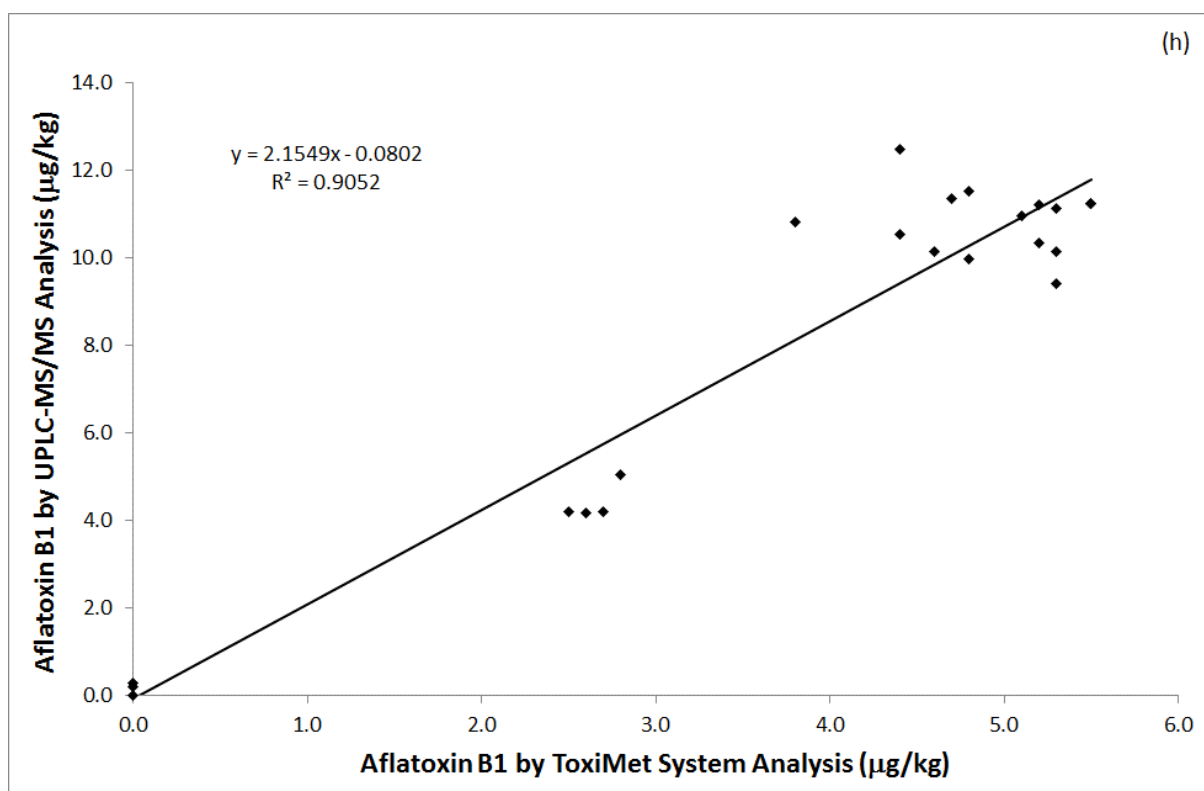
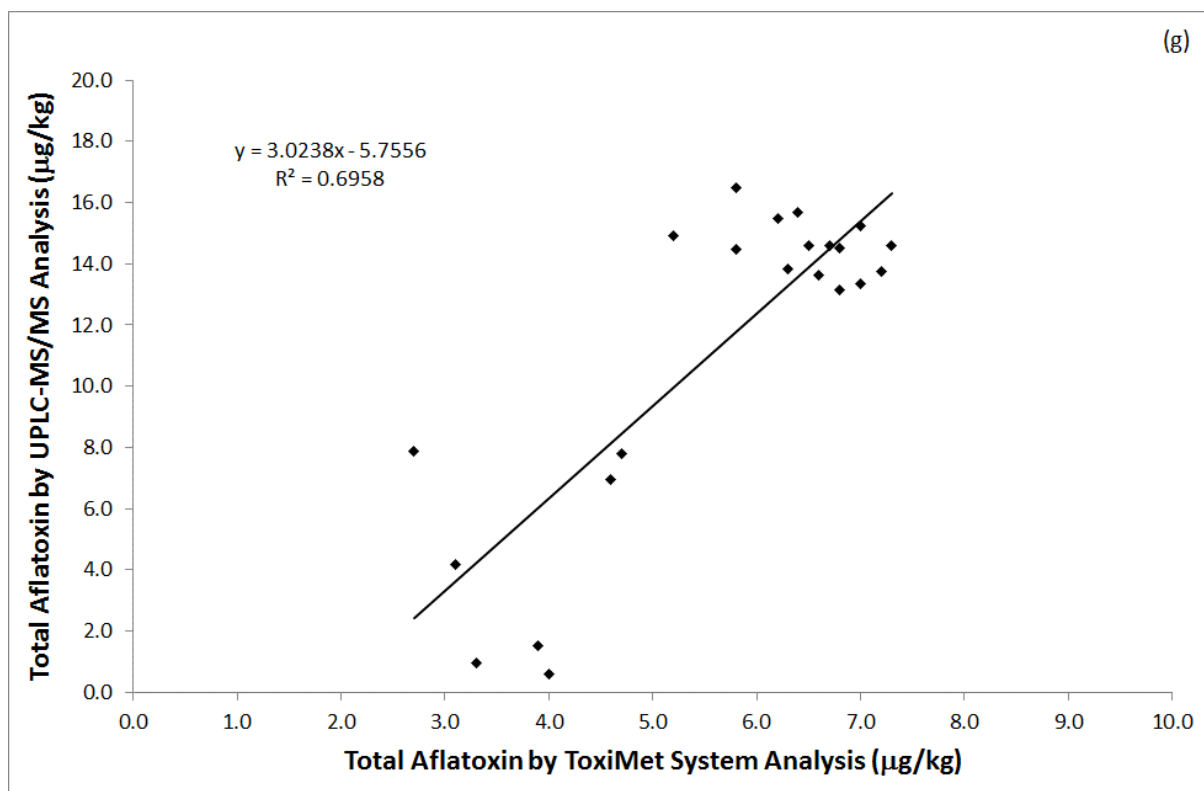


Table 1. The MS/MS conditions for aflatoxins analysis

Mycotoxin	Molecular weight	RT [min]	MRM transitions	Cone voltage [V]	Collision energy [eV]	Dwell time [ms]
Aflatoxin B1	312.3	5.0	313.2>285.0*	44	20	4
			313.2>241.2	44	36	4
Aflatoxin B2	314.3	4.7	315.1>287.1	68	24	4
			315.1>259.2	68	30	4
Aflatoxin G1	328.3	4.6	329.1>243.1	14	26	4
			329.1>200.0	14	36	4
Aflatoxin G2	330.3	4.4	331.1>245.1	12	28	5
			331.1>189.1	12	36	5
Aflatoxin M1	328.3	4.2	329.0>273.2	2	42	5
			329.0>229.1	2	22	5

* Transition in bold was used for quantification.

Table 2: Comparison of testing platforms showing the key attributes, benefits and limitations

Attribute	ToxiMet System	UPLC-MS/MS
Analysis	Aflatoxins B1, B2, G1 and G2	Aflatoxins B1, B2, G1, G2, M1 The current UPLC-MS/MS method operating in both positive and negative mode and requiring sample injection in two different mobile phases can detect a total of 79 mycotoxins
Sensitivity (ppb)	B1: LOD: 0.20 LOQ: 0.67 B2: LOD: 0.12 LOQ: 0.40 G1: LOD: 0.21 LOQ: 0.72 G2: LOD: 0.04 LOQ: 0.14	B1 LOD: 0.05, LOQ: 0.25 B2 LOD: 0.125, LOQ: 0.25 G1 LOD: 0.125, LOQ: 0.25 G2 LOD: 0.125, LOQ: 0.25 M1 LOD: 0.05, LOQ: 0.25
Specificity	Specific for Aflatoxins B1, B2, G1, G2,	Very specific for Aflatoxins B1, B2, G1, G2, M1 but method can be expanded to include a high number of mycotoxins for which standards were available
Ease of use	Method is relatively easy to use but requires initial training.	Skilled personnel with previous experience in LC-MS/MS methods and associated software for operation and interpretation of toxin profiles is required.
Amount of sample (g)	25	1
Sample Preparation	Sample Extraction with filter clean up ToxiSep Clean Up with filter clean up ToxiTrace Immobilisation	Sample Extraction using QuEChERS Centrifugation C18 Silica sorbent clean up Centrifugation Nitrogen Evaporation Filtering
Number of samples analysed in one round of preparation	20	30
Speed of analysis per sample	< 1 hour	5 hours
Speed of analysis for one round of samples	Toxin Extraction: 2.5 hr ToxiQuant Instrument Analysis: 0.45 hr Result Determination for 4 toxins: Immediate	Toxin Extraction: 4 hr Instrument Analysis: 19 hr aflatoxins only 38 hr all mycotoxins Result Determination: 2hr aflatoxins (including interpretation to the calibration curve)
Portability	May be applied outside the laboratory setting at different testing points along the food chain with basic facilities to allow for sample preparation	Not possible
Benefits	Relatively fast real time result, highly sensitive, highly specific multiplex analysis of four aflatoxins. There is no requirement for the purchase or preparation of analytical standards.	Accurate identification and quantification for compounds with available standards. Analytical standards grade or internal standards for aflatoxins are available but due to expense are not routinely used in analysis but are used for instrument calibration.
Limitations	Biosensor is relatively inexpensive requiring little maintenance and very limited training in use.	Equipment is highly expensive and requires substantial maintenance, requiring fully trained personnel for operation

Table 3: Range of aflatoxin concentrations determined by each method for each sample type

Sample Type	Method of Analysis	B1 (µg/kg)	B2 (µg/kg)	G1 (µg/kg)	G2 (µg/kg)	Total (µg/kg)	M1 (µg/kg)
Peanuts (n=71)	ToxiMet	0 - 178	0 - 10.6	0 - 47.9	0.12 - 11.1	0.23 - 204.0	N/A
	UPLC-MS/MS	0.63 - 4535	1.05 - 1098	0.72 - 2193	0.71 - 267.4	1.4 - 8094	0 - 381.1
Maize (n=79)	ToxiMet	0 - 57.9	0 - 8.5	0 - 39.3	0 - 8.9	0.01 - 114.6	N/A
	UPLC-MS/MS	0 - 80.5	0 - 7.0	0 - 83.6	0 - 3.8	0 - 172.7	0 - 5.3
Rice (n=88)	ToxiMet	0.16 - 12.4	0 - 2.9	0 - 8.8	0 - 1.9	0.15 - 26.0	N/A
	UPLC-MS/MS	0 - 14.1	0 - 1.1	0 - 16.6	0 - 0.9	0 - 32.7	0 - 0.8
Dried distillers grains (n=22)	ToxiMet	0-5.5	0-2.8	0-1.2	0.1-0.4	2.7-7.3	N/A
	UPLC-MS/MS	0-12.5	0-3.7	0-2.9	0-0.5	0.6-16.5	0 - 0.8

Table 4: Number of samples above the regulatory level by each method

Sample Type	Regulatory level	Number of samples above the regulatory levels by ToxiMet	Number of samples above the regulatory levels by UPLC-MS/MS
Rice (n=88)	B1 (>2 μ g/kg)	26 (29.5%)	21 (23.9%)
	Total (>4 μ g/kg)	16 (18.2%)	16 (18.2%)
Maize (n=79)	B1 (>2 μ g/kg)	40 (50.6%)	36 (45.6%)
	Total (>4 μ g/kg)	46 (58.2%)	40 (50.6%)
Peanuts (n=71)	B1 (>2 μ g/kg)	70 (98.6%)	70 (98.6%)
	Total (>4 μ g/kg)	70 (98.6%)	70 (98.6%)
Dried distillers grains (n=22)	B1 (>20 μ g/kg)	0	0