



**QUEEN'S
UNIVERSITY
BELFAST**

Development of peptide nucleic acid-based bead array technology for *Bacillus cereus* detection

Noppakudrittidej, P., Charlermroj, R., Makornwattana, M., Kaew-Amdee, S., Waditee-Sirisattha, R., Vilaivan, T., Praneenararat, T., & Karoonuthaisiri, N. (2023). Development of peptide nucleic acid-based bead array technology for *Bacillus cereus* detection. *Scientific Reports*, 13, Article 12482. Advance online publication. <https://doi.org/10.1038/s41598-023-38877-1>

Published in:
Scientific Reports

Document Version:
Publisher's PDF, also known as Version of record

Queen's University Belfast - Research Portal:
[Link to publication record in Queen's University Belfast Research Portal](#)

Publisher rights

Copyright 2023 The Authors.

This is an open access article published under a Creative Commons Attribution License (<https://creativecommons.org/licenses/by/4.0/>), which permits unrestricted use, distribution and reproduction in any medium, provided the author and source are cited.

General rights

Copyright for the publications made accessible via the Queen's University Belfast Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

The Research Portal is Queen's institutional repository that provides access to Queen's research output. Every effort has been made to ensure that content in the Research Portal does not infringe any person's rights, or applicable UK laws. If you discover content in the Research Portal that you believe breaches copyright or violates any law, please contact openaccess@qub.ac.uk.

Open Access

This research has been made openly available by Queen's academics and its Open Research team. We would love to hear how access to this research benefits you. – Share your feedback with us: <http://go.qub.ac.uk/oa-feedback>



OPEN

Development of peptide nucleic acid-based bead array technology for *Bacillus cereus* detection

Prae Noppakudrittidej^{1,2,3}, Rattaphol Charlermroj¹, Manlika Makornwattana¹, Suttida Kaew-amdee¹, Rungaroon Waditee-Sirisattha⁴, Tirayut Vilaivan^{2,5}, Thanit Praneenarat^{2,6}✉ & Nitsara Karoonuthaisiri^{1,6,7}✉

Numerous novel methods to detect foodborne pathogens have been extensively developed to ensure food safety. Among the important foodborne bacteria, *Bacillus cereus* was identified as a pathogen of concern that causes various food illnesses, leading to interest in developing effective detection methods for this pathogen. Although a standard method based on culturing and biochemical confirmative test is available, it is time- and labor-intensive. Alternative PCR-based methods have been developed but lack high-throughput capacity and ease of use. This study, therefore, attempts to develop a robust method for *B. cereus* detection by leveraging the highly specific pyrrolidinyl peptide nucleic acids (PNAs) as probes for a bead array method with multiplex and high-throughput capacity. In this study, PNAs bearing prolyl-2-aminocyclopentanecarboxylic acid (ACPC) backbone with *groEL*, *motB*, and *16S rRNA* sequences were covalently coupled with three sets of fluorescently barcoded beads to detect the three *B. cereus* genes. The developed acpcPNA-based bead array exhibited good selectivity where only signals were detectable in the presence of *B. cereus*, but not for other species. The sensitivity of this acpcPNA-based bead assay in detecting genomic DNA was found to be 0.038, 0.183 and 0.179 ng for *groEL*, *motB* and *16S rRNA*, respectively. This performance was clearly superior to its DNA counterpart, hence confirming much stronger binding strength of acpcPNA over DNA. The robustness of the developed method was further demonstrated by testing artificially spiked milk and pickled mustard greens with minimal interference from food matrices. Hence, this proof-of-concept acpcPNA-based bead array method has been proven to serve as an effective alternative nucleic acid-based method for foodborne pathogens.

Bacillus cereus is one of major foodborne pathogens that can be found in a wide range of food products ranging from ready-to-eat foods, fermented foods, and dairy products¹. Due to its tolerance to extreme pH and temperature, *B. cereus* was commonly found in various stages of food processing², resulting in serious foodborne outbreaks worldwide with an overall prevalence as high as 23.746%. In Europe, it is the second cause of the foodborne outbreak after *Staphylococcus aureus*³. In the USA, around 63,000 people/year got sick with 0.4% hospitalization rate from the *Bacillus* group⁴.

Rapid and accurate methods enabling timely monitoring and detection of *B. cereus* in food can serve as a key mitigation method in reducing its outbreaks. Moreover, given that not all species of *Bacillus* are pathogenic, it is imperative to be able to identify to the level of *Bacillus* species⁵. While a standard ISO 7932:2004 method is available based on agar plate-based counting protocol⁶, this method is time- and labor-consuming (requiring up to 24-h incubation period at 30 °C with an additional 2–7 days for confirmation assay), and requires trained professionals. Alternative molecular methods such as polymerase chain reaction (PCR)-based techniques have

¹National Center for Genetic Engineering and Biotechnology (BIOTEC), National Science and Technology Development Agency (NSTDA), Khlong Luang, Pathum Thani, Thailand 12120. ²Department of Chemistry, Faculty of Science, Chulalongkorn University, Phayathai Rd., Pathumwan, Bangkok, Thailand 10330. ³Program in Biotechnology, Faculty of Science, Chulalongkorn University, Phayathai Rd., Pathumwan, Bangkok, Thailand 10330. ⁴Department of Microbiology, Faculty of Science, Chulalongkorn University, Phayathai Rd., Pathumwan, Bangkok, Thailand 10330. ⁵Organic Synthesis Research Unit, Department of Chemistry, Faculty of Science, Chulalongkorn University, Phayathai Rd., Pathumwan, Bangkok, Thailand 10330. ⁶International Joint Research Center on Food Security, Khlong Luang, Pathum Thani, Thailand 12121. ⁷Institute for Global Food Security, Queen's University Belfast, Belfast, UK. ✉email: Thanit.P@chula.ac.th; nitsara.kar@biotec.or.th

been developed in order to identify *B. cereus*^{7,8}. However, most of these PCR-based methods rely on low-resolution gel electrophoresis methods to visualize PCR products, making them difficult for result interpretation. Many advanced PCR-based techniques such as quantitative PCR (qPCR) and multiplex PCR have therefore been developed to overcome these limitations^{9–11}, but their multiplex capacity is still limited due to complication from primer dimer formation¹². In addition, most PCR-based methods depend on DNA as a specific probe, which can be degraded by environmental factors, such as temperature, pH, and enzymes.

To overcome these limitations, this study showcases a detection method for *B. cereus* by combining the advantages of multiplex capacity and ease for result acquisition from bead array technique, and highly specific peptide nucleic acid (PNA) as an alternative probe. The bead array platform used in this study is based on a high-throughput, sensitive, and multiplex xMAP technology for different types of targets^{13,14}. This method utilizes paramagnetic fluorescently barcoded beads functionalized with carboxyl groups for covalent attachment of nucleophilic ligands. Each bead set can be identified by a red laser, and the signal is measured from a fluorescent reporter (R-phycoerythrin) by a green laser^{13,15,16}. Compared to traditional DNA microarray techniques, the bead array technology provides several advantages. First, the throughputness of this technique is clearly greater. This is because it is considered semi-automatic, while the DNA microarray technology is not. Second, owing to its automatic washing step, the bead array technology usually exhibits lower background and higher consistency than does the DNA microarray technology¹⁷. Lastly, the cost of a detector in the bead array technology is much cheaper than that of the DNA microarray, thus making it more practical. As such, various DNA-based bead array systems have been successfully applied for detecting a wide variety of food contaminations such as food allergens¹⁸, foodborne pathogens in chicken meat¹⁹ and four foodborne pathogens including *Salmonella* Typhimurium, *Brucella* spp., *B. cereus*, and *Shigella* spp. in dairy products²⁰. Interestingly, the reported method for *B. cereus* detection required elevated temperature at 38 °C to obtain detectable signal, likely due to less stability in DNA-DNA binding compared to PNA-DNA binding. This makes it impractical for actual industrial processing²⁰. Moreover, all of these reported bead array methods utilized DNA as a specific probe, whose specificity depends significantly on hybridization temperature and length of probes²¹. We surmised that the use of alternative nucleic acid mimics with better binding affinity to DNA target may improve overall sensing performance.

In this regard, PNA, a nucleic acid mimic in which the phosphodiester backbone has been replaced by pseudo-peptide backbone, was selected due to its various advantages such as high thermal stability, high sequence specificity, and high sensitivity for mismatch discrimination^{22–24}. Combined with the excellent stability of PNA toward nuclease and proteases, PNA has been developed for many applications including nucleic acid detection^{25–27}. The newer types of PNAs, such as conformationally constrained PNAs²⁸, were successfully developed to exhibit even better performance than does the original PNA (currently known as aegPNA). For example, Vilaivan and co-workers developed pyrrolidinyl PNA, which consists of nucleobase-modified proline and five-membered ring cyclic β -amino acids (named as acpcPNA)^{29,30}. This molecular feature avoids degradation under basic conditions from intermolecular cyclization – a fact of which happens readily with aegPNA consisting of α -amino acids³¹. Furthermore, acpcPNA has a more rigid structure than does aegPNA, leading to desirable properties such as better antiparallel selectivity, higher binding affinity, and better discrimination power toward single-base mismatch³². As such, acpcPNA has been utilized as a probe in DNA sensing studies involving various platforms^{33–37} such as paper-based sensors, surface plasmon resonance techniques, and electrochemical techniques.

To the best of our knowledge, never before has the Luminex bead array platform been combined with acpcPNA for foodborne pathogen detection. There was only one study that employed a similar concept of combining this Luminex bead array platform and aegPNA to improve detection capacity for detection of the *HER2* oncogene³⁸. Our developed method was demonstrated to exhibit good sensing performance with required robustness to detect *B. cereus* spiked in milk and pickled lettuce as models for real food samples. Hence, the developed method shows great promise to be adopted as a practical platform for the detection of *B. cereus* and the concept can be further applied for other pathogens in the future.

Materials and method

PNA synthesis. The sequences of acpcPNA probes used in this study are shown in Table 1. The PNA probes were synthesized with acetyl-capped N-terminus and the C-terminus modified with one lysine unit for conjugating with the carboxyl groups on the paramagnetic beads³⁹.

ID	Sequence (5'-3' for DNA and N-C for PNAs)
<i>groEL</i> PNA	Ac-GTAGGAAGCACAG-LysNH ₂
<i>motB</i> PNA	Ac-CGAACGTTAAGCC-LysNH ₂
<i>16S rRNA</i> PNA	Ac-AACGAGCGCAAC-LysNH ₂
<i>groEL</i> forward primer	CTGTAGTTGAAGGT
<i>groEL</i> reverse primer	Biotin-CACGAGTTGAGTT
<i>motB</i> forward primer	GTGAATGTATATCGA
<i>motB</i> reverse primer	Biotin-CTGCATATCCTAC
<i>16S rRNA</i> forward primer	Biotin-GTCGTCAGCTCGTGT
<i>16S rRNA</i> reverse primer	Biotin-CGATTACTAGCGATTCC

Table 1. acpcPNA and specific primer sequences used in this study.

Primer design. Primer sequences were designed by using Primer3 software (https://www.ncbi.nlm.nih.gov/tools/primer-blast/index.cgi?LINK_LOC=BlastHome) based on National Center for Biotechnology Information (NCBI) GenBank database as shown in Table 1.

Bacterial strains and media. Bacteria were obtained from Thailand Bioresource Research Center, Thailand (TBRC), American Type Culture Collection, United State of America (ATCC), and Department of Medical Sciences, Thailand (DMST) (Table 2). Except for *Bacillus* spp., all were streaked on a 2xYT agar plate (16 g/L tryptone, 10 g/L yeast extract, 5 g/L sodium chloride, and 15 g/L agar) and incubated at 37 °C for 16–18 h. A single colony of bacteria was inoculated in 10 mL of 2xYT broth (16 g/L tryptone, 10 g/L yeast extract, and 5 g/L sodium chloride) and incubated at 37 °C, 250 rpm for 16–18 h. *Bacillus* spp. were streaked on LB agar plates (10 g/L tryptone, 5 g/L yeast extract, 5 g/L sodium chloride, and 15 g/L agar) and incubated at 30 °C for 16–18 h. A single colony of *Bacillus* spp. was inoculated in 10 mL of LB broth (10 g/L tryptone, 5 g/L yeast extract, and 5 g/L sodium chloride) and cultured at 30 °C, 250 rpm for 16–18 h.

Genomic DNA extraction. Genomic DNA of each bacterial sample was extracted using a QIAamp®DNA Minikit (#51304, Qiagen) according to the user manual. In brief, bacterial cells were collected from a 1 mL sample by centrifugation at 7500 rpm for 5 min. The pellets were suspended in 180 µL of an enzyme solution (20 mg/mL lysozyme in 20 mM Tris–HCl, 2 mM EDTA, and 1.2% Triton-X 100) and incubated at 37 °C for 1 h. The pellets were treated with 20 µL of proteinase K at 56 °C for 2 h before being treated with 4 µL of RNase A (100 mg/mL) at room temperature for 2 min. The genomic DNA was further purified by a Qiagen mini spin column eluting with 50 µL of sterile water. Concentration and purity of the obtained genomic DNA were determined by UV-spectrophotometry (NanoDrop 8000 spectrophotometer, USA) at 260 and 280 nm.

Multiplex PCR amplification. Genomic DNA (50 ng) was used as a template in the polymerase chain reaction (PCR) to amplify the target amplicons using biotinylated primers. A PCR master mix solution included 1.25 U of Taq DNA polymerase (#M0273S, Biolabs), 50 mM of KCl, a mixture of three biotin-labeled primer sets, and 0.4 µM of dNTP (#N022, SibEnzyme). 35 cycles of PCR were performed using (1) denaturation at 95 °C for 30 s, (2) primer annealing at 52 °C for 30 s, and (3) DNA extension at 72 °C for 1 min. The biotinylated PCR products were analyzed by gel electrophoresis using 1.5% w/v agarose (#2125, OmniPur) in 0.5×TBE buffer (44.5 mM Tris, 44.5 mM Boric acid, and 1 mM EDTA) and SYBR®Safe. The images of the agarose gels were taken under UV light (302 nm), with size identification by a DNA ladder marker (100-base pairs, M25, SibEnzyme).

Development of bead array detection. *Bead conjugation with acpPNAs.* Three sets of fluorescently barcoded beads (#MC10012, #MC10015, #MC10021, Luminex) were coupled with three acpPNAs specific to *groEL*, *motB*, and *16S rRNA* genes. Each bead region (5×10^6 beads/region) was resuspended in 20 µL of 0.1 M MES, pH 4.5 (#M5057, Sigma) and linked with a specific acpPNA (0.1 nmol) and 2.5 µL of 10 mg/mL 1-ethyl-3-(3-dimethylaminopropyl) carbodiimide hydrochloride, (EDC-HCl, Thermo Fisher Scientific) for 30 min (in the dark). After this period, the second batch of EDC-HCl (2.5 µL of 10 mg/mL) was added to the reaction and incubated for another 30 min. The PNA-loaded beads were washed with 0.02% of Tween-20 (BioBasic inc.) and 0.1% SDS (BioBasic inc.) solution before reconstituted in 20 µL of TE buffer pH 8.0 (10 mM Tris–HCl, 0.1 mM EDTA) and kept at 4 °C in the dark until used.

Hybridization and detection. Three acpPNA-bead regions (2,500 beads/region/reaction, 33 µL each) were mixed together in 1.5×TMAC (4.5 M TMAC, 0.15% Sarkosyl solution, 75 mM Tris–HCl, and 6 mM EDTA, pH 8.0) and transferred to a 96 non-binding well plate (#655901, Greiner Bio-One). The biotinylated PCR product (10 µL) was added to TE buffer (7 µL), heated at 95 °C for 10 min and placed on ice rapidly for 3 min to maintain the DNA in single stranded form. For the hybridization step, the denatured PCR product solution was added to the bead mixture in the 96 non-binding well plate and incubated at 25 °C with shaking for 1 h before removing any unbound PCR products by washing three times with 100 µL of 1×TMAC buffer (3 M TMAC, 0.1% Sarkosyl solution, 50 mM Tris–HCl, and 4 mM EDTA, pH 8.0) with the aid of a magnetic separator plate. R-phycoerythrin-labeled streptavidin (25 µL of 10 µg/mL SAPE, #S866, Life technology™, USA.) in 1×TMAC buffer was added to the plate and incubated in a microplate shaker incubator (Hercuvan Lab systems, USA.) at 25 °C for 15 min. The plate was washed with 100 µL of 1×TMAC buffer for three times to remove unbound streptavidin

Bacterial strain	Source
<i>Bacillus cereus</i>	TBRC 4973
<i>B. subtilis</i>	TBRC 2901
<i>Escherichia coli</i>	ATCC 25322
<i>E. coli</i> O157: H7	DMST 12743
<i>Staphylococcus aureus</i>	ATCC 25923
<i>Salmonella</i> Enteritidis	ATCC 13076
<i>Salmonella</i> Typhimurium	ATCC 13311

Table 2. Bacterial strains used in this study.

before resuspended in 75 μL of MAGPIX Drive fluid (#40-50030, Luminex). Green laser in a Luminex instrument (MAGPIX™, Luminex, USA) was used to measure signal from reporter molecules at 525 nm. Red laser was used to identify specific bead set at 635 nm. Fluorescence signals from SAPE were measured and reported as median fluorescent intensity (MFI), which would be considered as a positive result when its value was at least 2 folds higher than the background or the negative control (distilled water as a template in PCR amplification).

Specificity, sensitivity, and the limit of detection. To evaluate specificity of the developed method, genomic DNA (50 ng) of six non-target foodborne pathogens (*B. subtilis*, *E. coli*, *E. coli* O157:H7, *Staphylococcus aureus*, *Salmonella* Enteritidis, and *Salmonella* Typhimurium) were used as templates in the PCR reactions. The PCR products were analyzed with the same PNA bead array using the same protocol as *B. cereus* described above (five replicates).

For sensitivity, different concentrations of genomic DNA (0.002–200 ng) of *B. cereus* were used as templates in PCR reactions and analyzed with the bead array (ten replicates).

The limit of detection (LOD) values were calculated as the concentration of genomic DNA with a signal greater than 2 folds of the background or the negative control (distilled water as a template in PCR amplification). The mean fluorescent intensity (MFI) signal were fitted to the following dose–response curve equation.

$$Y = A + (B/(1 + 10^{(C-X)}))$$

Y is a fluorescent intensity from RPE when detecting genomic DNA of pathogen concentration X. whereas A, B, and C are constants from curve fitting.

Performance comparison between DNA-based and acpcPNA-based bead array methods. Three specific DNA probes (0.1 nmol) with a hexyl spacer with equivalent sequences to those of acpcPNA were coupled with three beads regions (#MC10026, #MC10061, #MC10027, Luminex) via carbodiimide coupling as described in the section about bead conjugation with acpcPNAs. Thereafter, the DNA coupled beads were tested for sensitivity in detecting different concentrations of genomic DNA as described in sensitivity section.

Detection of *B. cereus* in artificially spiked food samples. To validate the developed method, artificially spiked food samples were tested. Two types of food samples (milk and pickled mustard greens) were collected from local supermarkets (12 samples per sample type). The samples were tested for the absence of *B. cereus* by the International Organization for Standardization 7932 (ISO 7932) method before the spiking experiment. Each *B. cereus*-free food sample (25 g) was homogenized with 225 mL of LB broth in sterile blender bags (#AES400/50G) for 2 min and spiked with *B. cereus* (10 CFU/mL in LB broth) followed by incubation at 30 °C for 16–18 h with 250 rpm shaking. Genomic DNA were extracted from the enriched food samples by a QIAamp®DNA Minikit as described in genomic DNA extraction section. The extracted DNA (2 μL) was used as a template for the PCR amplification and analyzed by the bead array as described above (three replicates).

Results and discussion

Design and optimization of acpcPNA-based bead array. To distinguish *B. cereus* from other species in the *Bacillus* groups (*B. anthracis*, *B. cereus*, *B. thuringiensis*, *B. mycoides*, *B. pseudomycoides*, and *B. weihenstephanensis*), chaperone *groEL* and mobility *motB* genes have previously been selected as robust biomarkers through bioinformatic method due to their unique sequences in *B. cereus* among other members of the genus³⁷. For internal control, the essential *16S rRNA* gene is selected due to its highly conserved sequence among the bacteria⁴⁰. Indeed, we have previously succeeded using acpcPNA of these genes as a specific probe and internal control in developing a highly specific and sensitive paper-based sensor to detect *B. cereus*³⁷. Importantly, while the paper-based platform is theoretically capable of multiplex analysis, the development of a paper-based sensing device with more than three gene targets is generally very tricky. On the other hand, a total of 50 gene targets can be included in one single assay well using bead array technology, thanks to its semi-automatic nature. Therefore, this study aims to develop a proof-of-concept acpcPNA-based bead array technology to empower the multiplex and high-throughput capacity of bead array platform for foodborne pathogen detection with superior specificity. Three fluorescently barcoded bead regions were linked with acpcPNA probes whose sequences match *groEL*, *motB*, and *16S rRNA* via the coupling between the carboxyl group on the bead and the amino group at the N-terminus of the PNA⁴¹ (Fig. 1A). The bead-immobilized acpcPNA probes were next hybridized with the biotinylated amplicons obtained from multiplex PCR via a strong Watson & Crick base pairing (Fig. 1B,C). This was followed by labeling of the bead-captured biotinylated DNA by an R-phycoerythrin-labeled streptavidin and the fluorescence intensities were measured by dual lasers (Fig. 1D,E).

To evaluate binding efficiency of synthesized acpcPNA sequences to their corresponding complementary DNAs, each type of acpcPNA-bead (*groEL*, *motB* and *16S rRNA*) was separately hybridized with its complementary DNA sequences (Fig. S1). The result indicated that the acpcPNAs were able to bind specifically to their complementary DNAs in all cases. This successful result can be attributed to the conformationally constraint nature of the PNA and the lack of negative charges on the backbone – both of which contributed to the strong binding affinity³². In addition, the combination of all three beads and their complementary DNA still showed clear fluorescence signals, albeit with slightly decreased intensities. This finding confirmed that this sensing system has potential for more complex studies.

Thereafter, a series of optimizations was performed to obtain as good performance as possible for hybridization experiments with amplicons, which are much larger in size than the complementary DNA strands. Key

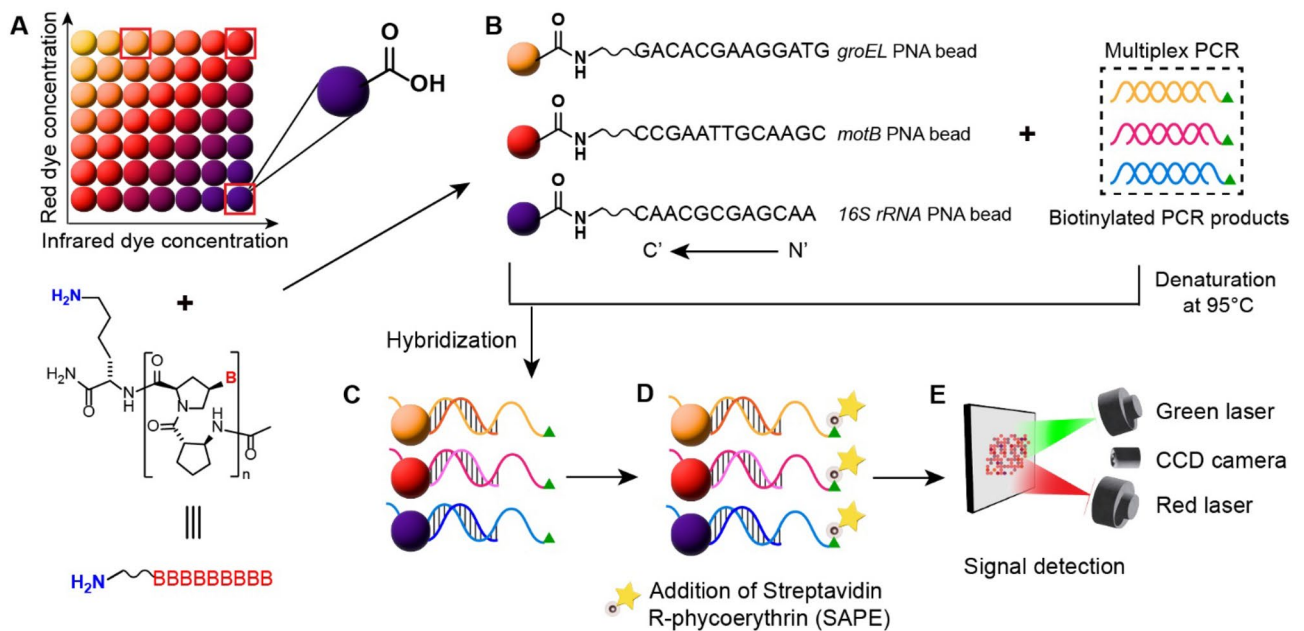


Figure 1. Schematic of acpcPNA-based bead array method. (A) A carboxyl group on each fluorescently barcoded paramagnetic bead allows covalent conjugation with the amino group on the acpcPNA molecule. (B) Three bead sets coupled with three specific acpcPNAs to *groEL*, *motB* and 16S *rRNA* genes were used to detect biotinylated PCR products from a multiplex PCR method. (C) Biotinylated single-stranded DNA after denatured at 95 °C was hybridized to acpcPNA-based beads. (D) R-phycoerythrin-labeled streptavidin (SAPE) molecules were bound to the biotin tag on the DNA-PNA bead complex. (E) A green laser was used to detect fluorescent signal from SAPE and a red laser was used to identify the region of bead set.

parameters to be optimized included hybridization time, concentrations of the reporter molecule (R-phycoerythrin-labeled streptavidin), and concentrations of primers. A range of hybridization times from 15 to 60 min were tested. As shown in Fig. S2, 30-min hybridization gave the highest signal to background ratio for *groEL* gene, while 60-min hybridization was the best for *motB* and 16S *rRNA* genes. Thus, 60 min of hybridization time was chosen. Also, Fig. S3 suggested that 10 µg/mL of the reporter molecule gave the best results, where the signal-to-background ratios were at 8.41, 4.06, and 2.44 for *groEL*, *motB*, and 16S *rRNA* genes, respectively. Lastly, since complication can arise from multiplex PCR, primer concentrations are also a key factor to be optimized. This was done by first focusing on the control gene (16S *rRNA*) primer as it likely dominates the amplification due to its high abundance in the genomic DNA template. Preliminary experiment suggested that 50 nM is the smallest concentration of the 16S *rRNA* primer that can still provide appreciable signal. Also, another separate experiment established that 1:2 amount ratio of *groEL*:*motB* primers provided the greatest signal intensity for simultaneous amplification using these two genes. Thereafter, we put these preliminary data together into the final optimization for multiplex PCR as shown in Fig. S4, where both the concentration of the 16S *rRNA* primer (at 50 nM), and the amount ratio of the *groEL* and *motB* primers (1:2) were held constant. That is, only the concentrations of *groEL* and *motB* primers were varied. The results suggested that, excluding the lowest concentrations tested, other conditions did not give significantly different outcomes. Hence, the second lowest concentrations of primers seemed to be the most logical choice. However, this condition (300:600:50 nM of *groEL*, *motB*, and 16S *rRNA* primers, respectively) could not result in appreciable amplifications in other tested bacterial species. Thus, the concentrations of 400:800:50 nM of *groEL*, *motB*, and 16S *rRNA* primers, respectively, were instead selected for subsequent studies.

Evaluation of sensing performance. Specificity of the developed method was evaluated against seven relevant foodborne species namely *B. cereus*, *B. subtilis*, *Escherichia coli*, *E. coli* O157:H7, *Staphylococcus aureus*, *Salmonella* Enteritidis, and *Salmonella* Typhimurium. In each case, the isolated genomic DNA was used as a template for the multiplex PCR amplification with biotin tagging to all three target genes and tested by the acpcPNA-based bead array. In the case of *B. cereus* detection, both *groEL* and *motB* beads exhibited positive results with the highest signal from the *groEL* bead at approximately 7 folds of signal-to-background ratio (Fig. 2). The signals from *groEL* and *motB* beads for other tested bacteria were negative, while the internal positive control from the 16S *rRNA* beads were positive in all bacteria species, thus confirming that this gene can be employed as a robust internal control for this sensing platform.

Overall, while the signals obtained from the detection of longer DNA amplicons (200–310 bp) were lower than those obtained from short synthetic DNA oligonucleotides (Fig. S1), the results are sufficient for unambiguous identification of *B. cereus*. This decrease in signal intensity is unsurprising because amplicons used herein are 200–310 bp, which are much longer than probe sequences on the solid support (12–15 bp). Given the chance of forming secondary structures from DNA in this length^{16,42}, the results are considered to be decent. Moreover,

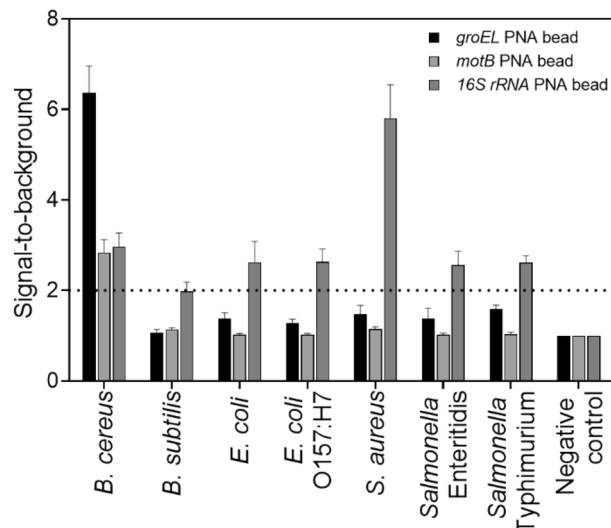


Figure 2. Specificity of the acpcPNA-based bead array detection against *B. cereus*, *B. subtilis*, *E. coli*, *E. coli* O157:H7, *S. aureus*, *Salmonella* Enteritidis, and *Salmonella* Typhimurium. Genomic DNA sample (50 ng) of each species was tested. Each data group was plotted as an average of five-replicates with an error bar that indicated a standard deviation. The dotted line represents a cut-off value which is two times of the intensity from negative control. The negative control had water as a template for amplification.

the lower signal could be from the complication of multiplex PCR amplicons. The increased number of primer sets for multiple targets within a single reaction could generate spurious amplification products due to formation of primer dimer⁴³.

The limit of detection (LOD) of this method was evaluated for all genes used in detecting known genomic DNA concentrations (Fig. 3A). A clear increase of fluorescent intensities was shown around 0.1 ng, where signal started to rise in a linear fashion up to around 1 ng before reaching a plateau¹⁶. The *groEL* PNA bead was able to detect as low as 0.038 ng of genomic DNA, while the *motB* and *16S rRNA* beads gave LOD values of 0.183 and 0.179 ng of genomic DNA, respectively. The obtained LOD values are less sensitive than our previous paper-based sensor³⁷ which could be due to the use of multiplex PCR which is known to be more complicated to develop and often less sensitive than conventional PCR⁴⁴. However, the multiplex capacity of this developed method and the ease of a single step multiplex PCR offer an important advancement of the detection method as it can further include detection of other important genes such as emetic toxin genes from *B. cereus* strains⁴² and specific genes for other bacteria. Importantly, the superior performance of acpcPNA over DNA was also proven by evaluating the sensing performance of DNA probes having the same sequences as the acpcPNA probes used in this study (Fig. 3B). Interestingly, while the LOD of *groEL* DNA bead was comparable to its acpcPNA counterpart (0.032 ng vs 0.038 ng respectively), the signal from the *groEL* DNA bead seemed to reach somewhat higher plateau, i.e., higher signal-to-background ratio, at much higher amount of genomic DNA sample (~ 30 ng) than did the acpcPNA bead. Nonetheless, the *motB* and *16S rRNA* DNA beads could not detect genomic DNA in any amounts of genomic DNA tested (Fig. 3B). This could be explained by the low stability of the duplexes formed between the relatively short DNA probes and the DNA target. The results confirm the superior performance of acpcPNA over DNA probes in terms of robustness in the multiplex assay.

Assay performance in real matrices. *B. cereus* outbreaks have been reported in various foods, such as starchy foods and rice, raw and processed vegetables, bread, milk and dairy products, meat products, and ready-to-eat foods^{2,3}. To validate the developed method, two types of food matrices namely milk and pickled mustard greens were selected to represent dairy products and ready-to-eat foods. The food samples were confirmed to be free of *B. cereus* by the ISO 7932 method before spiking experiments. The *B. cereus*-free milk and pickled mustard greens (n = 12 per each food matrix) were spiked with 10 CFU/g of *B. cereus*. This figure is lower than the maximum acceptable number of *B. cereus* (10² CFU/mL and 50 CFU/g for children under the age of 6 months) according to the Codex Alimentarius Commission of the Food and Agriculture Organization of the United Nations (FAO) and the World Health Organization (WHO)⁴⁵. Thereafter, the spiked samples were enriched by incubation at 30 °C overnight, followed by genomic DNA extraction. The biotinylated PCR products were prepared by multiplex PCR under the optimal condition obtained previously, and the amounts of the DNA target sequence for the three genes were measured by the acpcPNA-based bead array. The culture media with 10 CFU/g of *B. cereus* was used as a positive control. There were three types of negative controls in this study to cover all possibilities including the use of distilled water as a template for PCR amplification, and the use of unspiked matrices for DNA purification prior to PCR amplification. Gratifyingly, the developed assay was able to identify three specific genes of *B. cereus* with little interference of the food matrix (Fig. 4). The *groEL* bead again provided the highest signal in both matrices. The lower signals obtained from pickled mustard greens are likely due to the presence of various inhibitors such as enzymes, polysaccharides, proteins, and salt, all of which could interfere

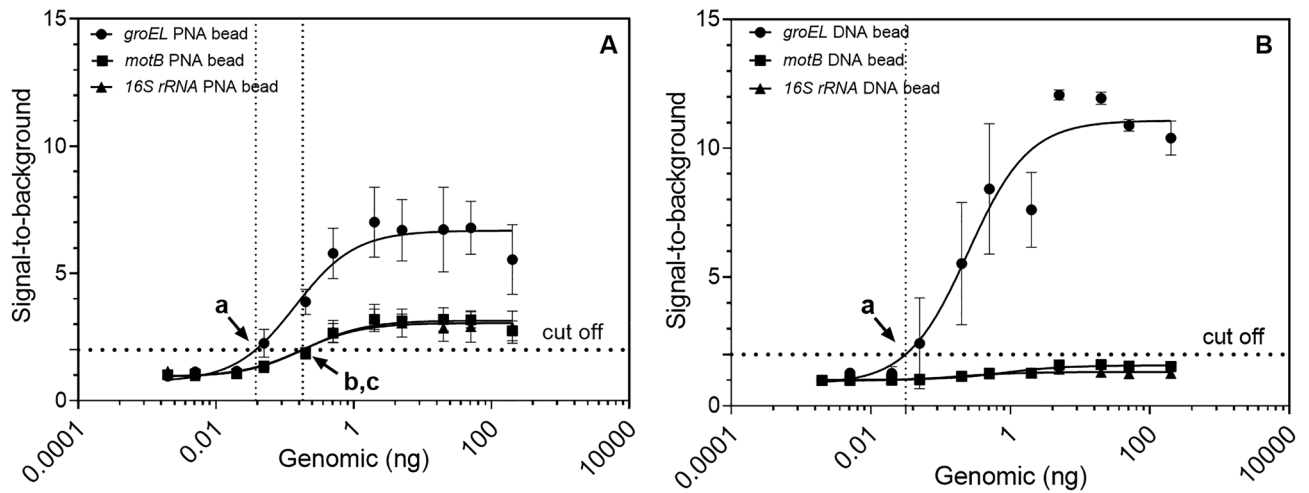


Figure 3. Responses of (A) acpPNA-based arrays (LOD = 0.038 ng (a), 0.183 ng (b), and 0.179 ng (c) of genomic DNA for *groEL*, *motB*, and *16S rRNA* PNA beads, respectively), and (B) DNA-based bead arrays (LOD = 0.032 ng (a) for *groEL* DNA bead). Each data point was plotted as an average of ten replicates with an error bar that indicated a standard deviation. The dotted line at the bottom of the graph represents a cut-off value which is two times the intensity from the negative control.




Figure 4. The acpPNA-based bead array used to detect *B. cereus* in artificially spiked food samples. *B. cereus* (10 CFU/mL) was spiked into milk, pickled mustard greens, and positive control (culture media). Each data group was plotted as an average of 12 samples with an error bar that indicated a standard deviation. The dotted line represents a cut-off value which is two times of the intensity from the negative control (water as a template in the PCR amplification).

with genomic DNA extraction and subsequent PCR amplification⁹. Nevertheless, the data from real food matrices clearly demonstrated that the developed acpPNA-based bead array can be adopted as an alternative method for specific and multiplex detection for foodborne pathogens.

Conclusion

In this study, we successfully developed a multiplex acpPNA-based bead array technique to identify *Bacillus cereus* with good specificity, low limit of detection, and high-throughput capacity. The total assay time of 4 h, including multiplex PCR amplification, is shorter than the culture-based ISO method which requires at least 72 h to identify *B. cereus*. The validation of the developed method with representative real food matrices indicates that our method can detect the prevalent *B. cereus* pathogen accurately and its practicality can further be explored for food safety support in industrial processes.

Data availability

The datasets analyzed during the current study are available in the GenBank repository, [*groEL* Gene ID: 72447092; *motB* Gene ID: 72451176; *16S rRNA* Nucleotide ID: NR_074540.1].

Received: 26 April 2023; Accepted: 17 July 2023

Published online: 01 August 2023

References

- Zhang, Z. *et al.* Detection of viable enterotoxin-producing *Bacillus cereus* and analysis of toxigenicity from ready-to-eat foods and infant formula milk powder by multiplex PCR. *J. Dairy Sci.* **99**, 1047–1055 (2016).
- Rahnama, H., Azari, R., Hashem, M. & Berizi, E. A systematic review and meta-analysis of the prevalence of *Bacillus cereus* in foods. *Food Control* **143**, 109250 (2023).
- Glasset, B. *et al.* *Bacillus cereus*-induced food-borne outbreaks in France, 2007 to 2014: Epidemiology and genetic characterisation. *Eurosurveillance* **21**, 30413 (2016).
- Carroll, L. M. *et al.* Characterization of emetic and diarrheal *Bacillus cereus* strains from a 2016 foodborne outbreak using whole-genome sequencing: Addressing the microbiological, epidemiological, and bioinformatic challenges. *Front. Microbiol.* **10**, 144 (2019).
- Frentzel, H. *et al.* Phylogenetic and toxinogenic characteristics of *Bacillus cereus* group members isolated from spices and herbs. *Food Control* **83**, 90–98 (2018).
- United States. *Bacteriological Analytical Manual*, vol 1 (Association of Official Analytical Chemists (Chapter 14), 1978).
- Wei, S. *et al.* Molecular discrimination of *Bacillus cereus* group species in foods (lettuce, spinach, and kimchi) using quantitative real-time PCR targeting *groEL* and *gyrB*. *Microb. Pathog.* **115**, 312–320 (2018).
- Chang, Y.-H., Shangkuang, Y.-H., Lin, H.-C. & Liu, H.-W. PCR assay of the *groEL* gene for detection and differentiation of *Bacillus cereus* group cells. *Appl. Environ. Microbiol.* **69**, 4502–4510 (2003).
- Forghani, F., Singh, P., Seo, K. H. & Oh, D. H. A novel pentaplex real time (RT)-PCR high resolution melt curve assay for simultaneous detection of emetic and enterotoxin producing *Bacillus cereus* in food. *Food Control* **60**, 560–568 (2016).
- Frentzel, H., Kelner-Burgos, Y. & Deneke, C. Evaluation of a real-time PCR assay for the differentiation of *Bacillus cereus* group species. *Food Control* **120**, 107530 (2021).
- Yossa, N. *et al.* qPCR detection of viable *Bacillus cereus* group cells in cosmetic products. *Sci. Rep.* **13**, 4477 (2023).
- Zhao, X., Lin, C. W., Wang, J. & Oh, D. H. Advances in rapid detection methods for foodborne pathogens. *J. Microbiol. Biotechnol.* **24**, 297–312 (2014).
- Dunbar, S. A. & Li, D. Introduction to Luminex® xMAP® technology and applications for biological analysis in China. *Asia Pac. Biotech* **14**, 26–30 (2010).
- Reslova, N., Huvarova, V., Hrdy, J., Kasny, M. & Kralik, P. A novel perspective on MOL-PCR optimization and MAGPIX analysis of in-house multiplex foodborne pathogens detection assay. *Sci. Rep.* **9**, 5842 (2019).
- Karoonthaisiri, N. *et al.* Bead array for *Listeria monocytogenes* detection using specific monoclonal antibodies. *Food Control* **47**, 462–471 (2015).
- Sun, Z. *et al.* Simultaneous and highly sensitive detection of six different foodborne pathogens by high-throughput suspension array technology. *Food Control* **40**, 300–309 (2014).
- Charlarmroj, R. *et al.* Multiplex detection of plant pathogens using a microsphere immunoassay technology. *PLoS One* **8**, e62344 (2013).
- Nowatzke, W. L., Oliver, K. G., Cho, C. Y., Rallabhandi, P. & Garber, E. A. E. Single-laboratory validation of the multiplex xMAP food allergen detection assay with incurred food samples. *J. Agric. Food Chem.* **67**, 484–498 (2019).
- Charlarmroj, R. *et al.* DNA-based bead array technology for simultaneous identification of eleven foodborne pathogens in chicken meat. *Food Control* **101**, 81–88 (2019).
- Shi, Y. *et al.* Establishment of a method for the simultaneous detection of four foodborne pathogens using high-throughput suspension array xTAG technology. *Int. J. Food Sci. Technol.* **54**, 2578–2585 (2019).
- Livshits, M. A. & Mirzabekov, A. D. Theoretical analysis of the kinetics of DNA hybridization with gel-immobilized oligonucleotides. *Biophys. J.* **71**, 2795–2801 (1996).
- Nielsen, P. E., Egholm, M., Berg, R. H. & Buchardt, O. Sequence-selective recognition of DNA by strand displacement with a Thymine-substituted polyamide. *Science* **254**, 1497–1500 (1991).
- Nielsen, P. E. Peptide nucleic acid. A molecule with two identities. *Acc. Chem. Res.* **32**, 624–630 (1999).
- Siddiquee, S., Rovina, K. & Azriah, A. A review of peptide nucleic acid. *Adv. Tech. Biol. Med.* **3**, 1000131 (2015).
- Wang, J. PNA biosensors for nucleic acid detection. *Curr. Issues Mol. Biol.* **1**, 117–122 (1999).
- Vilaivan, T. Fluorogenic PNA probes. *Beilstein J. Org. Chem.* **14**, 253–281 (2018).
- Lai, Q., Chen, W., Zhang, Y. & Liu, Z. Application strategies of peptide nucleic acids toward electrochemical nucleic acid sensors. *Analyst* **146**, 5822–5835 (2021).
- Suparpprom, C. & Vilaivan, T. Perspectives on conformationally constrained peptide nucleic acid (PNA): Insights into the structural design, properties and applications. *RSC Chem. Biol.* **3**, 648–697 (2022).
- Vilaivan, T., Suparpprom, C., Harnyuttanakorn, P. & Lowe, G. Synthesis and properties of novel pyrrolidinyl PNA carrying β -amino acid spacers. *Tetrahedron Lett.* **42**, 5533–5536 (2001).
- Vilaivan, T. & Srisuwannaket, C. Hybridization of pyrrolidinyl peptide nucleic acids and DNA: Selectivity, base-pairing specificity, and direction of binding. *Org. Lett.* **8**, 1897–1900 (2006).
- Thomson, S. A. *et al.* Fmoc mediated synthesis of peptide nucleic acids. *Tetrahedron* **51**, 6179–6194 (1995).
- Vilaivan, T. Pyrrolidinyl PNA with α/β -dipeptide backbone: From development to applications. *Acc. Chem. Res.* **48**, 1645–1656 (2015).
- Ananthanawat, C., Vilaivan, T., Hoven, V. P. & Su, X. Comparison of DNA, aminoethylglycyl PNA and pyrrolidinyl PNA as probes for detection of DNA hybridization using surface plasmon resonance technique. *Biosens. Bioelectron.* **25**, 1064–1069 (2010).
- Jampasa, S. *et al.* Electrochemical detection of human papillomavirus DNA type 16 using a pyrrolidinyl peptide nucleic acid probe immobilized on screen-printed carbon electrodes. *Biosens. Bioelectron.* **54**, 428–434 (2014).
- Teengam, P. *et al.* Multiplex paper-based colorimetric DNA sensor using pyrrolidinyl peptide nucleic acid-induced AgNPs aggregation for detecting MERS-CoV, MTB, and HPV oligonucleotides. *Anal. Chem.* **89**, 5428–5435 (2017).
- Jirakittiwut, N. *et al.* Visual genotyping of thalassemia by using pyrrolidinyl peptide nucleic acid probes immobilized on carboxymethylcellulose-modified paper and enzyme-induced pigmentation. *Microchim. Acta* **187**, 238 (2020).
- Jirakittiwut, N. *et al.* Paper-based sensor from pyrrolidinyl peptide nucleic acid for the efficient detection of *Bacillus cereus*. *Anal. Bioanal. Chem.* **413**, 6661–6669 (2021).
- Metaferia, B. *et al.* Development of peptide nucleic acid probes for detection of the *HER2* oncogene. *PLoS One* **8**, e58870 (2013).
- Vilaivan, T. & Srisuwannaket, C. Hybridization of pyrrolidinyl peptide nucleic acids and DNA: Selectivity, base-pairing specificity, and direction of binding. *Org. Lett.* **8**, 1897–1900 (2006).
- Clarridge, J. E. Impact of *16S rRNA* gene sequence analysis for identification of bacteria on clinical microbiology and infectious diseases. *Clin. Microbiol. Rev.* **17**, 840–862 (2004).
- Jirakittiwut, N., Panyain, N., Nuanyai, T., Vilaivan, T. & Praneenarat, T. Pyrrolidinyl peptide nucleic acids immobilised on cellulose paper as a DNA sensor. *RSC Adv.* **5**, 24110–24114 (2015).
- Ehling-Schulz, M., Fricker, M. & Scherer, S. Identification of emetic toxin producing *Bacillus cereus* strains by a novel molecular assay. *FEMS Microbiol. Lett.* **232**, 189–195 (2004).
- Elnifro, E. M., Ashshi, A. M., Cooper, R. J. & Klapper, P. E. Multiplex PCR: Optimization and application in diagnostic virology. *Clin. Microbiol. Rev.* **13**, 559–570 (2000).

44. Shen, C. H. Amplification of nucleic acids. In *Diagnostic Molecular Biology* (ed. Shen, C.-H.) 215–247 (Academic Press, 2019). <https://doi.org/10.1016/B978-0-12-802823-0.00009-2>.
45. Cormontagne, D. *et al.* *Bacillus cereus* induces severe infections in preterm neonates: Implication at the hospital and human milk bank level. *Toxins* **13**, 123 (2021).

Acknowledgements

The authors thank the National Center for Genetic Engineering and Biotechnology (BIOTEC) and Chulalongkorn University—NSTDA Doctoral Scholarship, The 90th Anniversary of Chulalongkorn University Scholarship, and the Overseas Research Experience Scholarship for graduate students for financial support. This research also received funding support from the NRSF via the Program Management Unit for Human Resources & Institutional Development, Research and Innovation (grant number PMU-B: B16F640114).

Author contributions

P.N. conducted all laboratory experiments in this study. R.C. helped in some experiments and gave advice on several aspects of the study. M.M. provided supports in PCR experiments and bioinformatic analysis. S.K. provided support in bead array experiments. R.W. provided support in bioinformatic analysis. T.V. provided support in PNA chemistry. T.P. and N.K. wrote the manuscript, and supervised all research activities.

Competing interests

The authors declare no competing interests.

Additional information

Supplementary Information The online version contains supplementary material available at <https://doi.org/10.1038/s41598-023-38877-1>.

Correspondence and requests for materials should be addressed to T.P. or N.K.

Reprints and permissions information is available at www.nature.com/reprints.

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2023